

LB107066

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AK

Instrument ID : Konelab

1/7/2020 13:47

Test: Total CN

ug/L

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	93.709	0.0	0.098	
ICB1	0.737	0.0	0.003	
CCV1	239.826	0.0	0.248	
CCB1	0.604	0.0	0.002	
PB125932BL	0.455	0.0	0.002	
L1017-03	0.236	0.0	0.002	
L1017-03DUP	0.356	0.0	0.002	
L1039-03	0.374	0.0	0.002	
L1039-04	0.558	0.0	0.002	
L1039-07	0.378	0.0	0.002	
L1039-08	0.283	0.0	0.002	
L1039-09	0.096	0.0	0.002	
CCV2	254.736	0.0	0.263	
CCB2	0.624	0.0	0.002	

N	14
Mean	42.355
SD	90.3307
CV%	213.27

AK

Aquakem v. 7.2AQ1

Results from time period:

Tue Jan 07 13:38:10 2020

Tue Jan 07 13:42:03 2020

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive	CI P	0.1276	µg/l	1/7/2020 9:18:35	
5.OPPBCN	A	Reactive	CI P	5.325	µg/l	1/7/2020 9:18:36	
10PPBCN	A	Reactive	CI P	10.1222	µg/l	1/7/2020 9:18:37	
50PPBCN	A	Reactive	CI P	49.6672	µg/l	1/7/2020 9:18:38	
100PPBCN	A	Reactive	CI P	100.2307	µg/l	1/7/2020 9:18:39	
250PPBCN	A	Reactive	CI P	249.0916	µg/l	1/7/2020 9:18:40	
500PPBCN	A	Reactive	CI P	500.4357	µg/l	1/7/2020 9:18:41	
ICV1	S	Reactive	CI P	93.7091	µg/l	1/7/2020 13:38:10	
ICB1	S	Reactive	CI P	0.7368	µg/l	1/7/2020 13:38:11	
CCV1	S	Reactive	CI P	239.826	µg/l	1/7/2020 13:38:12	
CCB1	S	Reactive	CI P	0.6035	µg/l	1/7/2020 13:38:13	
PB125932BL	S	Reactive	CI P	0.455	µg/l	1/7/2020 13:38:14	
L1017-03	S	Reactive	CI P	0.2357	µg/l	1/7/2020 13:38:15	
L1017-03DUP	S	Reactive	CI P	0.3562	µg/l	1/7/2020 13:38:16	
L1039-03	S	Reactive	CI P	0.3738	µg/l	1/7/2020 13:38:17	
L1039-04	S	Reactive	CI P	0.5581	µg/l	1/7/2020 13:38:18	
L1039-07	S	Reactive	CI P	0.3779	µg/l	1/7/2020 13:38:19	
L1039-08	S	Reactive	CI P	0.2833	µg/l	1/7/2020 13:38:20	
L1039-09	S	Reactive	CI P	0.0956	µg/l	1/7/2020 13:42:01	
CCV2	S	Reactive	CI P	254.7358	µg/l	1/7/2020 13:42:02	
CCB2	S	Reactive	CI P	0.6245	µg/l	1/7/2020 13:42:03	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AL

Instrument ID : Konelab

1/7/2020 13:32

Test Total CN


Accepted 1/7/2020 9:25

Factor 973.5

Bias 0.002

Coeff. of det. 0.999994

Errors

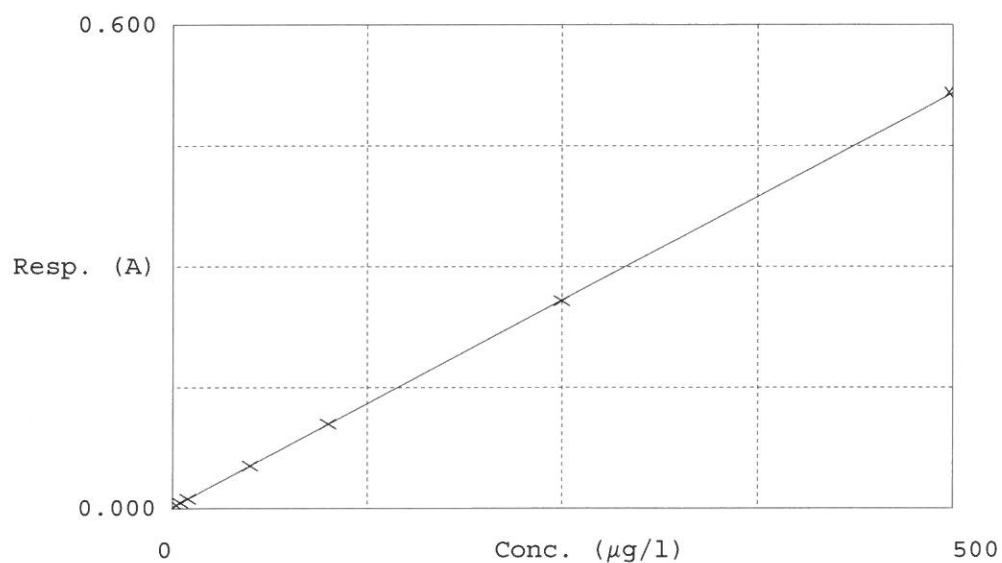

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	0.1276	0.0000	
2	5.0PPBCN	0.007	5.3250	5.0000	
3	10PPBCN	0.012	10.1222	10.0000	
4	50PPBCN	0.053	49.6672	50.0000	
5	100PPBCN	0.105	100.2307	100.0000	
6	250PPBCN	0.258	249.0916	250.0000	
7	500PPBCN	0.516	500.4357	500.0000	