

C8107114

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

Instrument ID : Konelab

1/10/2020 11:21

Test: ^{Reactive} ~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.076	0.0	0.098	
ICB1	0.399	0.0	0.003	
CCV1	240.114	0.0	0.248	
CCB1	0.260	0.0	0.002	
PB125967BL	0.150	0.0	0.002	
L1060-06	-0.106	0.0	0.002	
L1060-06DUP	-0.041	0.0	0.002	
L1060-12	0.028	0.0	0.002	
L1060-18	0.190	0.0	0.002	
L1064-03	0.151	0.0	0.002	
L1064-07	0.207	0.0	0.002	
L1064-10	-0.119	0.0	0.002	
L1065-01	0.088	0.0	0.002	
L1070-03	0.199	0.0	0.002	
CCV2	246.485	0.0	0.254	
CCB2	0.184	0.0	0.002	
L1070-06	-0.043	0.0	0.002	
CCV3	247.874	0.0	0.256	
CCB3	0.133	0.0	0.002	

N	19
Mean	43.696
SD	92.0217
CV%	210.59

Aquakem v. 7.2AQ1

Results from time period:

Fri Jan 10 10:03:52 2020

AK

Fri Jan 10 11:14:42 2020

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive	CI P	-0.2441	µg/l	1/10/2020 10:03:52	
5.OPPBCN	A	Reactive	CI P	4.8884	µg/l	1/10/2020 10:03:53	
10PPBCN	A	Reactive	CI P	9.869	µg/l	1/10/2020 10:03:54	
50PPBCN	A	Reactive	CI P	50.1345	µg/l	1/10/2020 10:03:55	
100PPBCN	A	Reactive	CI P	99.3011	µg/l	1/10/2020 10:03:56	
250PPBCN	A	Reactive	CI P	251.8423	µg/l	1/10/2020 10:03:57	
500PPBCN	A	Reactive	CI P	499.2089	µg/l	1/10/2020 10:03:58	
ICV1	S	Reactive	CI P	94.0759	µg/l	1/10/2020 11:08:24	
ICB1	S	Reactive	CI P	0.3993	µg/l	1/10/2020 11:08:25	
CCV1	S	Reactive	CI P	240.1138	µg/l	1/10/2020 11:08:26	
CCB1	S	Reactive	CI P	0.2598	µg/l	1/10/2020 11:08:27	
PB125967BL	S	Reactive	CI P	0.1498	µg/l	1/10/2020 11:08:28	
L1060-06	S	Reactive	CI P	-0.1058	µg/l	1/10/2020 11:08:29	
L1060-06DUP	S	Reactive	CI P	-0.0414	µg/l	1/10/2020 11:08:30	
L1060-12	S	Reactive	CI P	0.0275	µg/l	1/10/2020 11:08:31	
L1060-18	S	Reactive	CI P	0.1903	µg/l	1/10/2020 11:08:32	
L1064-03	S	Reactive	CI P	0.1513	µg/l	1/10/2020 11:08:33	
L1064-07	S	Reactive	CI P	0.2069	µg/l	1/10/2020 11:08:34	
L1064-10	S	Reactive	CI P	-0.1189	µg/l	1/10/2020 11:14:35	
L1065-01	S	Reactive	CI P	0.0884	µg/l	1/10/2020 11:14:36	
L1070-03	S	Reactive	CI P	0.1993	µg/l	1/10/2020 11:14:37	
CCV2	S	Reactive	CI P	246.485	µg/l	1/10/2020 11:14:38	
CCB2	S	Reactive	CI P	0.1843	µg/l	1/10/2020 11:14:39	
L1070-06	S	Reactive	CI P	-0.0428	µg/l	1/10/2020 11:14:40	
CCV3	S	Reactive	CI P	247.8742	µg/l	1/10/2020 11:14:41	
CCB3	S	Reactive	CI P	0.1332	µg/l	1/10/2020 11:14:42	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AL

Instrument ID : Konelab

1/10/2020 10:09

Test Total CN


Accepted 1/10/2020 10:09

Factor 977.9

Bias 0.002

Coeff. of det. 0.999978

Errors

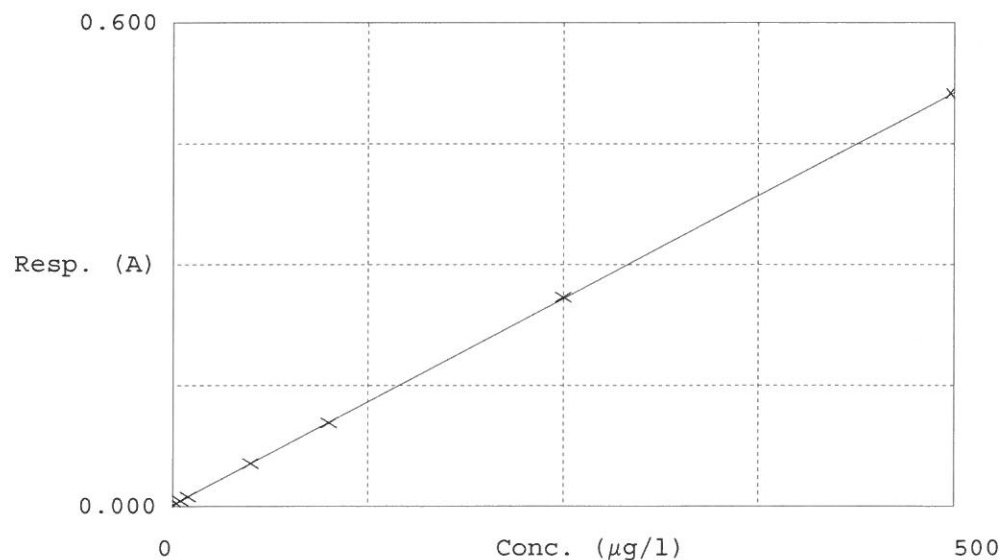

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	-0.2441	0.0000	
2	5.0PPBCN	0.007	4.8884	5.0000	
3	10PPBCN	0.012	9.8690	10.0000	
4	50PPBCN	0.053	50.1345	50.0000	
5	100PPBCN	0.104	99.3011	100.0000	
6	250PPBCN	0.260	251.8423	250.0000	
7	500PPBCN	0.513	499.2089	500.0000	