

LB107122

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AK

Instrument ID : Konelab

1/10/2020 13:13

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.390	0.0	0.100	
ICB1	0.001	0.0	0.002	
CCV1	240.594	0.0	0.248	
CCB1	0.336	0.0	0.002	
PB125961BL	0.322	0.0	0.002	
PB125961BS	95.425	0.0	0.100	
LOWPB125961	9.613	0.0	0.012	
HIGHPB125961	485.509	0.0	0.499	
L1060-01	1.303	0.0	0.003	
L1060-01DUP	1.176	0.0	0.003	
L1060-01MS	31.759	0.0	0.035	
L1060-07	0.953	0.0	0.003	
L1060-13	1.662	0.0	0.004	
CCV2	241.459	0.0	0.249	
CCB2	0.373	0.0	0.003	
L1064-01	0.197	0.0	0.002	
L1064-05	0.458	0.0	0.003	
L1070-01	0.553	0.0	0.003	
L1070-04	0.918	0.0	0.003	
L1084-01	3.065	0.0	0.005	
L1084-02	7.038	0.0	0.009	
L1084-03	4.335	0.0	0.007	
L1060-01MSD	32.821	0.0	0.036	
CCV3	271.660	0.0	0.280	
CCB3	0.055	0.0	0.002	

N	25
Mean	61.079
SD	121.2626
CV%	198.53

Aquakem v. 7.2AQ1

Results from time period:

Fri Jan 10 12:17:02 2020

Fri Jan 10 13:09:44 2020

PC

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	-0.2441	µg/l	1/10/2020 10:03:52	
5.OPPBCN	A	Total CN	P	4.8884	µg/l	1/10/2020 10:03:53	
10PPBCN	A	Total CN	P	9.869	µg/l	1/10/2020 10:03:54	
50PPBCN	A	Total CN	P	50.1345	µg/l	1/10/2020 10:03:55	
100PPBCN	A	Total CN	P	99.3011	µg/l	1/10/2020 10:03:56	
250PPBCN	A	Total CN	P	251.8423	µg/l	1/10/2020 10:03:57	
500PPBCN	A	Total CN	P	499.2089	µg/l	1/10/2020 10:03:58	
ICV1	S	Total CN	P	95.3898	µg/l	1/10/2020 12:17:02	
ICB1	S	Total CN	P	0.0007	µg/l	1/10/2020 12:17:03	
CCV1	S	Total CN	P	240.5941	µg/l	1/10/2020 12:17:04	
CCB1	S	Total CN	P	0.3359	µg/l	1/10/2020 12:17:05	
PB125961BL	S	Total CN	P	0.3221	µg/l	1/10/2020 12:17:06	
PB125961BS	S	Total CN	P	95.4252	µg/l	1/10/2020 12:17:07	
LOWPB125961	S	Total CN	P	9.6128	µg/l	1/10/2020 12:17:08	
HIGHPB125961	S	Total CN	P	485.5095	µg/l	1/10/2020 12:17:09	
L1060-01	S	Total CN	P	1.3027	µg/l	1/10/2020 12:17:10	
L1060-01DUP	S	Total CN	P	1.176	µg/l	1/10/2020 12:17:11	
L1060-01MS	S	Total CN	P	31.7594	µg/l	1/10/2020 12:17:12	
L1060-07	S	Total CN	P	0.9531	µg/l	1/10/2020 12:24:36	
L1060-13	S	Total CN	P	1.6621	µg/l	1/10/2020 12:24:37	
CCV2	S	Total CN	P	241.4593	µg/l	1/10/2020 12:24:38	
CCB2	S	Total CN	P	0.3726	µg/l	1/10/2020 12:24:39	
L1064-01	S	Total CN	P	0.1966	µg/l	1/10/2020 12:24:40	
L1064-05	S	Total CN	P	0.4576	µg/l	1/10/2020 12:24:41	
L1070-01	S	Total CN	P	0.5535	µg/l	1/10/2020 12:24:42	
L1070-04	S	Total CN	P	0.9181	µg/l	1/10/2020 12:24:43	
L1084-01	S	Total CN	P	3.0646	µg/l	1/10/2020 12:24:44	
L1084-02	S	Total CN	P	7.0384	µg/l	1/10/2020 12:24:45	
L1084-03	S	Total CN	P	4.3352	µg/l	1/10/2020 12:28:54	
L1060-01MSD	S	Total CN	P	32.8207	µg/l	1/10/2020 12:54:40	
CCV3	S	Total CN	P	271.6605	µg/l	1/10/2020 13:09:43	
CCB3	S	Total CN	P	0.0548	µg/l	1/10/2020 13:09:44	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AL

Instrument ID : Konelab

1/10/2020 13:37


Test Total CN

Accepted 1/10/2020 10:09

Factor 977.9
Bias 0.002

Coeff. of det. 0.999978

Errors

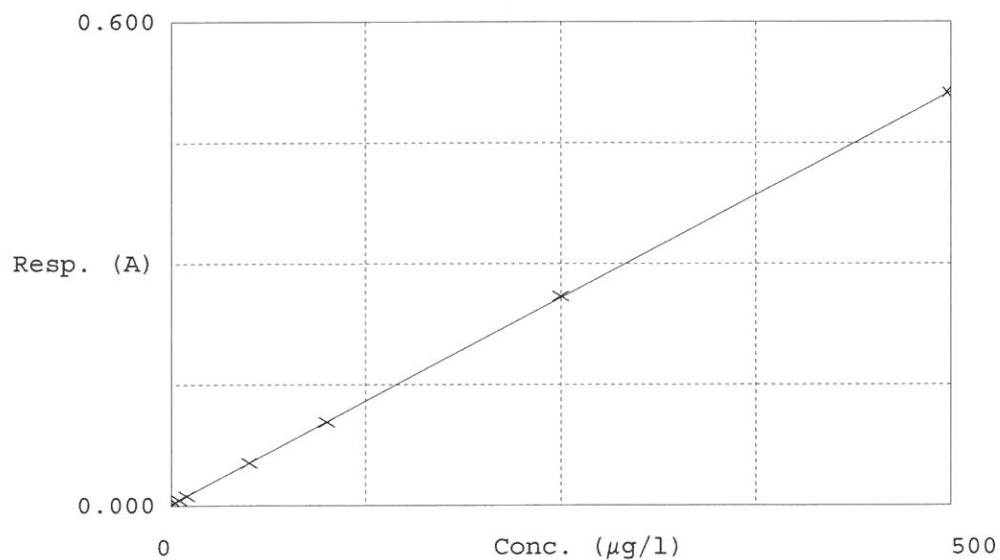

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	-0.2441	0.0000	
2	5.0PPBCN	0.007	4.8884	5.0000	
3	10PPBCN	0.012	9.8690	10.0000	
4	50PPBCN	0.053	50.1345	50.0000	
5	100PPBCN	0.104	99.3011	100.0000	
6	250PPBCN	0.260	251.8423	250.0000	
7	500PPBCN	0.513	499.2089	500.0000	