

68107143

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AK

Instrument ID : Konelab

1/13/2020 14:19

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.745	0.0	0.099	
ICB1	0.396	0.0	0.002	
CCV1	249.858	0.0	0.258	
CCB1	0.300	0.0	0.002	
PB126042BL	0.077	0.0	0.002	
PB126042BS	94.963	0.0	0.099	
MIDPB126042	244.953	0.0	0.253	
L1102-01	0.515	0.0	0.003	
L1102-01DUP	0.510	0.0	0.003	
L1102-01MS	31.528	0.0	0.034	
L1102-01MSD	32.357	0.0	0.035	
CCV2	259.326	0.0	0.267	
CCB2	0.142	0.0	0.002	

N	13
Mean	77.667
SD	104.6022
CV%	134.68

AK

Aquakem v. 7.2AQ1

Results from time period:

Mon Jan 13 13:58:31 2020

Mon Jan 13 14:19:09 2020

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	-0.1113	µg/l	1/13/2020 10:55:48	
5.OPPBCN	A	Total CN	P	5.1198	µg/l	1/13/2020 10:55:49	
10PPBCN	A	Total CN	P	10.001	µg/l	1/13/2020 10:55:50	
50PPBCN	A	Total CN	P	49.3341	µg/l	1/13/2020 10:55:51	
100PPBCN	A	Total CN	P	99.7678	µg/l	1/13/2020 10:55:52	
250PPBCN	A	Total CN	P	251.5534	µg/l	1/13/2020 10:55:53	
500PPBCN	A	Total CN	P	499.3351	µg/l	1/13/2020 10:55:54	
ICV1	S	Total CN	P	94.7449	µg/l	1/13/2020 13:58:31	
ICB1	S	Total CN	P	0.3956	µg/l	1/13/2020 13:58:32	
CCV1	S	Total CN	P	249.8578	µg/l	1/13/2020 13:58:33	
CCB1	S	Total CN	P	0.3002	µg/l	1/13/2020 13:58:34	
PB126042BL	S	Total CN	P	0.0771	µg/l	1/13/2020 13:58:35	
PB126042BS	S	Total CN	P	94.9627	µg/l	1/13/2020 13:58:36	
MIDPB126042	S	Total CN	P	244.9535	µg/l	1/13/2020 13:58:37	
L1102-01	S	Total CN	P	0.5152	µg/l	1/13/2020 13:58:38	
L1102-01DUP	S	Total CN	P	0.5097	µg/l	1/13/2020 13:58:39	
L1102-01MS	S	Total CN	P	31.5285	µg/l	1/13/2020 13:58:40	
L1102-01MSD	S	Total CN	P	32.3566	µg/l	1/13/2020 14:17:17	
CCV2	S	Total CN	P	259.3256	µg/l	1/13/2020 14:17:18	
CCB2	S	Total CN	P	0.1417	µg/l	1/13/2020 14:19:09	

LB107143

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092

Reviewed by : AL

Instrument ID : Konelab

1/13/2020 10:56

Test Total CN


Accepted 1/13/2020 10:56

Factor 977.5

Bias 0.002

Coeff. of det. 0.999984

Errors

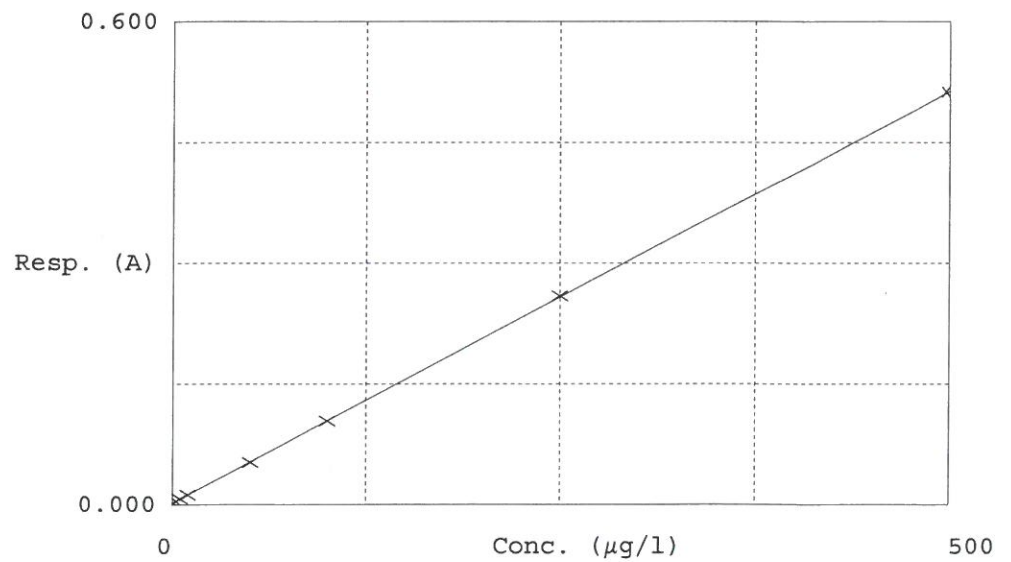

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	-0.1113	0.0000	
2	5.0PPBCN	0.007	5.1198	5.0000	
3	10PPBCN	0.012	10.0010	10.0000	
4	50PPBCN	0.053	49.3341	50.0000	
5	100PPBCN	0.104	99.7678	100.0000	
6	250PPBCN	0.259	251.5534	250.0000	
7	500PPBCN	0.513	499.3351	500.0000	