

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by :

Instrument ID : Konelab

1/14/2020 15:47

Test: ~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.174	0.0	0.095	
ICB1	0.402	0.0	0.003	
CCV1	244.138	0.0	0.243	
CCB1	0.265	0.0	0.002	
PB126081BL	0.168	0.0	0.002	
L1004-03	0.013	0.0	0.002	
L1004-03DUP	-0.053	0.0	0.002	
L1004-06	-0.193	0.0	0.002	
L1004-09	-0.025	0.0	0.002	
L1111-02	-0.040	0.0	0.002	
L1111-05	-0.130	0.0	0.002	
L1111-08	0.245	0.0	0.002	
CCV2	261.351	0.0	0.260	
CCB2	0.321	0.0	0.002	

N	14
Mean	42.903
SD	92.4071
CV%	215.39

Aquakem v. 7.2AQ1

Results from time period:

Tue Jan 14 15:42:50 2020

Tue Jan 14 15:46:43 2020

AK

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive	Cl P	-0.0625	µg/l	1/14/2020 13:07:59	
5.OPPBCN	A	Reactive	Cl P	5.2394	µg/l	1/14/2020 13:08:00	
10PPBCN	A	Reactive	Cl P	10.1235	µg/l	1/14/2020 13:08:01	
50PPBCN	A	Reactive	Cl P	48.9418	µg/l	1/14/2020 13:08:02	
100PPBCN	A	Reactive	Cl P	99.3032	µg/l	1/14/2020 13:08:03	
250PPBCN	A	Reactive	Cl P	252.4287	µg/l	1/14/2020 13:08:04	
500PPBCN	A	Reactive	Cl P	499.026	µg/l	1/14/2020 13:08:05	
ICV1	S	Reactive	Cl P	94.1742	µg/l	1/14/2020 15:42:50	
ICB1	S	Reactive	Cl P	0.4022	µg/l	1/14/2020 15:42:51	
CCV1	S	Reactive	Cl P	244.138	µg/l	1/14/2020 15:42:52	
CCB1	S	Reactive	Cl P	0.2651	µg/l	1/14/2020 15:42:53	
PB126081BL	S	Reactive	Cl P	0.1682	µg/l	1/14/2020 15:42:54	
L1004-03	S	Reactive	Cl P	0.0128	µg/l	1/14/2020 15:42:55	
L1004-03DUP	S	Reactive	Cl P	-0.0528	µg/l	1/14/2020 15:42:56	
L1004-06	S	Reactive	Cl P	-0.1931	µg/l	1/14/2020 15:42:57	
L1004-09	S	Reactive	Cl P	-0.0245	µg/l	1/14/2020 15:42:58	
L1111-02	S	Reactive	Cl P	-0.0396	µg/l	1/14/2020 15:42:59	
L1111-05	S	Reactive	Cl P	-0.1296	µg/l	1/14/2020 15:43:00	
L1111-08	S	Reactive	Cl P	0.2453	µg/l	1/14/2020 15:46:41	
CCV2	S	Reactive	Cl P	261.3508	µg/l	1/14/2020 15:46:42	
CCB2	S	Reactive	Cl P	0.3208	µg/l	1/14/2020 15:46:43	

CB107163

=====

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AK

Instrument ID : Konelab

1/14/2020 13:21


Test Total CN

Accepted 1/14/2020 13:21

Factor 1014
Bias 0.002

Coeff. of det. 0.999959

Errors

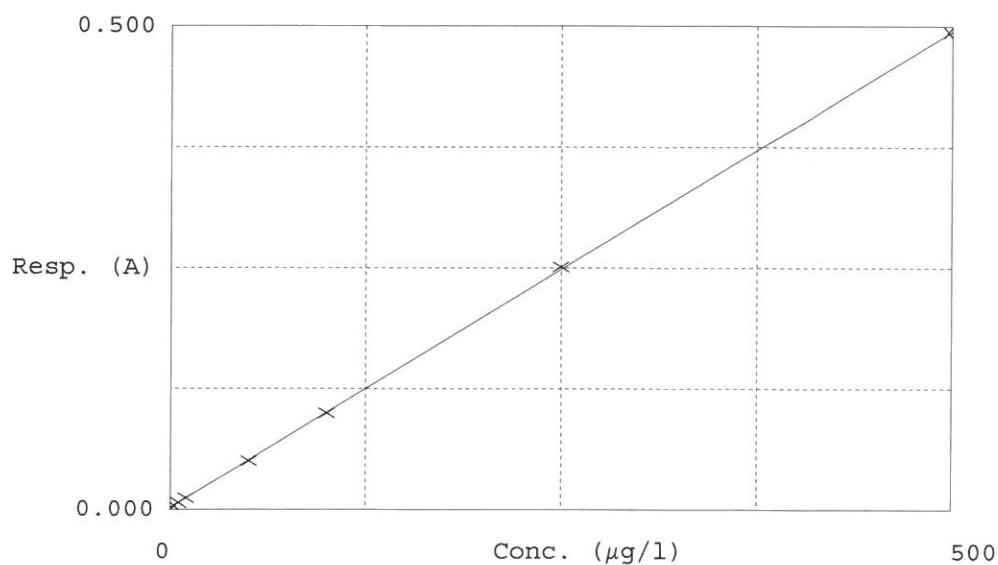

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	-0.0625	0.0000	
2	5.0PPBCN	0.007	5.2394	5.0000	
3	10PPBCN	0.012	10.1235	10.0000	
4	50PPBCN	0.050	48.9418	50.0000	
5	100PPBCN	0.100	99.3032	100.0000	
6	250PPBCN	0.251	252.4287	250.0000	
7	500PPBCN	0.494	499.0260	500.0000	