

LB107209

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

Instrument ID : Konelab

1/16/2020 13:23

Test: ~~Total~~ ^{Reactive} CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.206	0.0	0.101	
ICB1	0.512	0.0	0.003	
CCV1	240.550	0.0	0.254	
CCB1	-0.205	0.0	0.002	
PB126111BL	0.118	0.0	0.002	
L1005-05	0.001	0.0	0.002	
L1006-04	0.071	0.0	0.002	
L1016-09	0.004	0.0	0.002	
L1017-06	0.028	0.0	0.002	
L1123-09	-0.219	0.0	0.002	
L1123-10	-0.079	0.0	0.002	
L1123-11	-0.023	0.0	0.002	
L1123-12	0.169	0.0	0.002	
CCV2	244.464	0.0	0.258	
CCB2	0.809	0.0	0.003	
L1126-06	0.010	0.0	0.002	
L1005-05DUP	0.282	0.0	0.003	
CCV3	254.898	0.0	0.269	
CCB3	0.248	0.0	0.003	

N	19
Mean	43.992
SD	92.7078
CV%	210.74

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

Instrument ID : Konelab

1/16/2020 10:14


Test Total CN

Accepted 1/16/2020 10:14

Factor 956.4
Bias 0.002

Coeff. of det. 0.999998

Errors

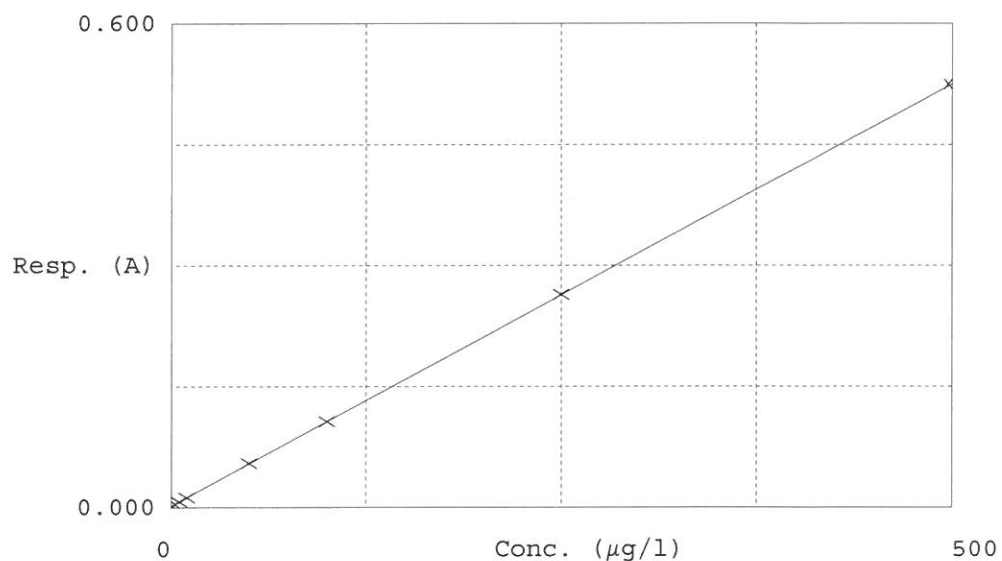

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	-0.0494	0.0000	
2	5.0PPBCN	0.007	4.8671	5.0000	
3	10PPBCN	0.013	9.7951	10.0000	
4	50PPBCN	0.055	50.2648	50.0000	
5	100PPBCN	0.107	99.8975	100.0000	
6	250PPBCN	0.264	250.4509	250.0000	
7	500PPBCN	0.525	499.7740	500.0000	

AL

Aquakem v. 7.2AQ1

Results from time period:

Thu Jan 16 10:14:31 2020

Thu Jan 16 13:18:19 2020

Sample Id	Sam/Ctr/c/	Test short Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive Cl P	-0.0494	µg/l	1/16/2020 10:14:31	
5.OPPBCN	A	Reactive Cl P	4.8671	µg/l	1/16/2020 10:14:32	
10PPBCN	A	Reactive Cl P	9.7951	µg/l	1/16/2020 10:14:33	
50PPBCN	A	Reactive Cl P	50.2648	µg/l	1/16/2020 10:14:34	
100PPBCN	A	Reactive Cl P	99.8975	µg/l	1/16/2020 10:14:35	
250PPBCN	A	Reactive Cl P	250.4509	µg/l	1/16/2020 10:14:36	
500PPBCN	A	Reactive Cl P	499.774	µg/l	1/16/2020 10:14:37	
ICV1	S	Reactive Cl P	94.2058	µg/l	1/16/2020 12:58:13	
ICB1	S	Reactive Cl P	0.5122	µg/l	1/16/2020 12:58:14	
CCV1	S	Reactive Cl P	240.5498	µg/l	1/16/2020 12:58:15	
CCB1	S	Reactive Cl P	-0.2047	µg/l	1/16/2020 12:58:16	
PB126111BL	S	Reactive Cl P	0.1185	µg/l	1/16/2020 12:58:17	
L1005-05	S	Reactive Cl P	0.0015	µg/l	1/16/2020 12:58:18	
L1006-04	S	Reactive Cl P	0.0708	µg/l	1/16/2020 12:58:20	
L1016-09	S	Reactive Cl P	0.0045	µg/l	1/16/2020 12:58:21	
L1017-06	S	Reactive Cl P	0.028	µg/l	1/16/2020 12:58:22	
L1123-09	S	Reactive Cl P	-0.2186	µg/l	1/16/2020 12:58:23	
L1123-10	S	Reactive Cl P	-0.0786	µg/l	1/16/2020 13:04:27	
L1123-11	S	Reactive Cl P	-0.0231	µg/l	1/16/2020 13:04:28	
L1123-12	S	Reactive Cl P	0.1688	µg/l	1/16/2020 13:04:29	
CCV2	S	Reactive Cl P	244.4641	µg/l	1/16/2020 13:04:30	
CCB2	S	Reactive Cl P	0.8092	µg/l	1/16/2020 13:04:31	
L1126-06	S	Reactive Cl P	0.0098	µg/l	1/16/2020 13:04:32	
L1005-05DUP	S	Reactive Cl P	0.2822	µg/l	1/16/2020 13:18:17	
CCV3	S	Reactive Cl P	254.898	µg/l	1/16/2020 13:18:18	
CCB3	S	Reactive Cl P	0.2484	µg/l	1/16/2020 13:18:19	