

03107235

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AR

Instrument ID : Konelab

1/17/2020 14:16

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.012	0.0	0.118	
ICB1	-0.002	0.0	0.008	
CCV1	0.980	0.0	0.114	
CCB1	0.001	0.0	0.009	
PB126140BL	0.000	0.0	0.008	
PB126140BS	1.031	0.0	0.120	
L1123-13	-0.000	0.0	0.008	
L1123-13DUP	-0.003	0.0	0.008	
L1123-13MS	0.967	0.0	0.113	
L1123-13MSD	0.965	0.0	0.113	
L1142-02	0.020	0.0	0.011	
CCV2	0.975	0.0	0.114	
CCB2	-0.001	0.0	0.008	

N	13
Mean	0.457
SD	0.5120
CV%	111.97

Aquakem v. 7.2AQ1

Results from time period:

Fri Jan 17 13:09:38 2020

Fri Jan 17 14:11:32 2020

AK

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0474	mg/l	1/17/2020 13:09:38	
0.1PPM	A	Phenolics-	P	0.102	mg/l	1/17/2020 13:09:39	
0.25PPM	A	Phenolics-	P	0.2495	mg/l	1/17/2020 13:09:40	
0.50PPM	A	Phenolics-	P	0.5	mg/l	1/17/2020 13:09:41	
1.0PPM	A	Phenolics-	P	1.0021	mg/l	1/17/2020 13:09:42	
2.0PPM	A	Phenolics-	P	1.999	mg/l	1/17/2020 13:09:43	
ICV1	S	Phenolics-	P	1.0116	mg/l	1/17/2020 13:49:12	
ICB1	S	Phenolics-	P	-0.002	mg/l	1/17/2020 13:49:13	
CCV1	S	Phenolics-	P	0.9801	mg/l	1/17/2020 13:49:14	
CCB1	S	Phenolics-	P	0.0011	mg/l	1/17/2020 13:49:15	
PB126140BL	S	Phenolics-	P	0.0002	mg/l	1/17/2020 13:49:16	
PB126140BS	S	Phenolics-	P	1.0308	mg/l	1/17/2020 13:49:17	
L1123-13	S	Phenolics-	P	-0.0003	mg/l	1/17/2020 13:49:18	
L1123-13DUP	S	Phenolics-	P	-0.0035	mg/l	1/17/2020 13:49:19	
L1123-13MS	S	Phenolics-	P	0.9673	mg/l	1/17/2020 13:49:20	
L1123-13MSD	S	Phenolics-	P	0.9648	mg/l	1/17/2020 13:49:21	
L1142-02	S	Phenolics-	P	0.0202	mg/l	1/17/2020 13:49:22	
CCV2	S	Phenolics-	P	0.975	mg/l	1/17/2020 13:49:23	
CCB2	S	Phenolics-	P	-0.0007	mg/l	1/17/2020 13:52:00	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : ph

Instrument ID : Konelab

1/17/2020 13:20


Test Phenolics-

Accepted 1/17/2020 13:20

Factor 9.266
Bias 0.008

Coeff. of det. 0.999994

Errors

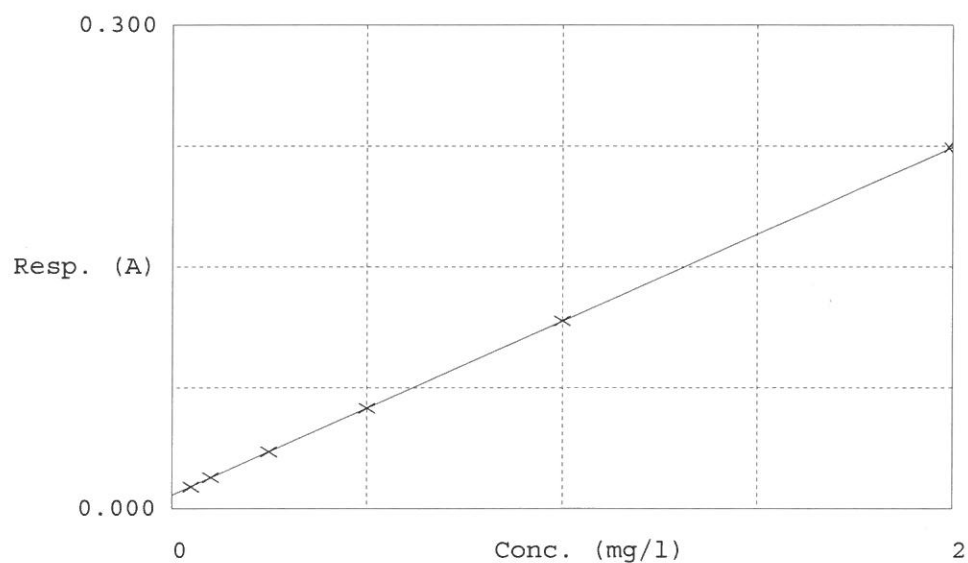

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.014	0.0474	0.0500	
2	Phenol-2	0.019	0.1020	0.1000	
3	Phenol-2	0.035	0.2495	0.2500	
4	Phenol-2	0.062	0.5000	0.5000	
5	Phenol-2	0.117	1.0021	1.0000	
6	Phenol-2	0.224	1.9990	2.0000	