


LB107262

Instrument ID: CV1

7470A

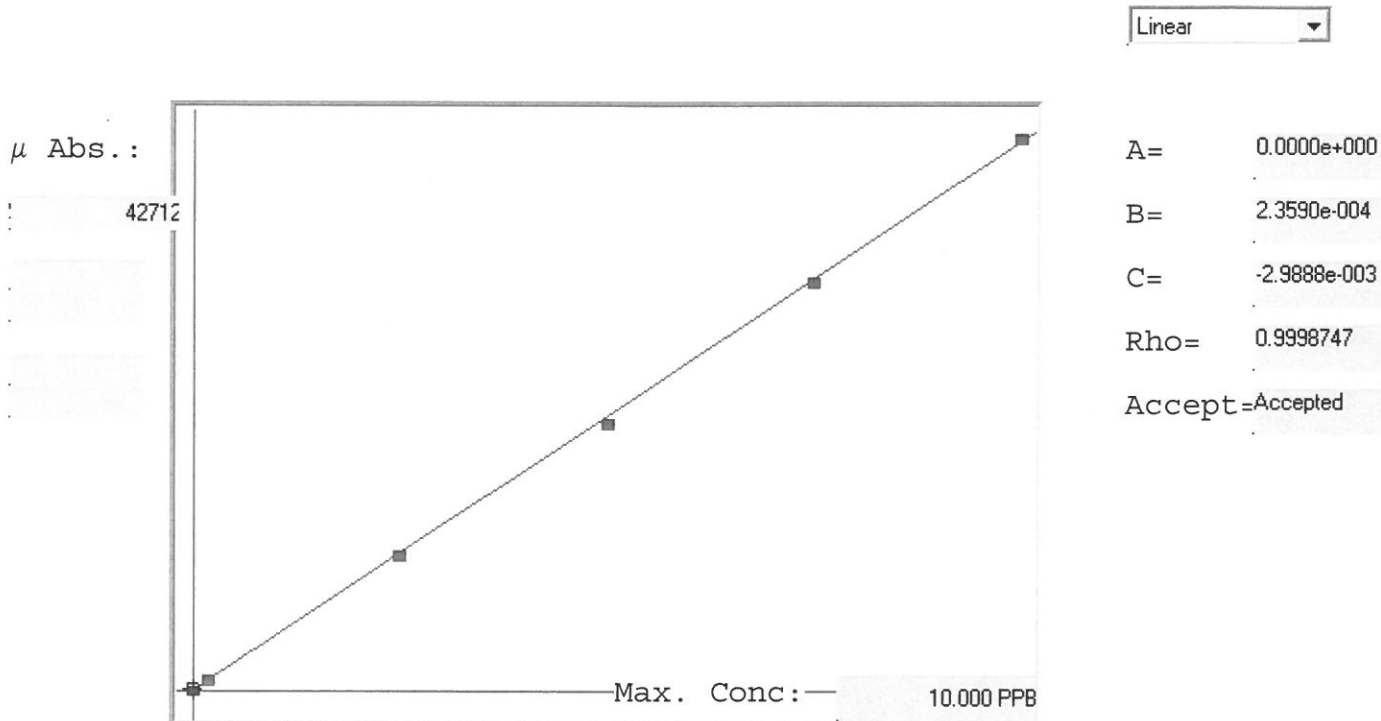

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.041	0.041	186	0.000	186				
0.2	0.200	0.234	0.034	1004	0.0 %	1004				
2.5	2.500	2.483	-0.017	10540	0.0 %	10540				
5.0	5.000	4.893	-0.107	20753	0.0 %	20753				
7.5	7.500	7.476	-0.024	31706	0.0 %	31706				
10.0	10.000	10.073	0.073	42712	0.0 %	42712				

LB107262 INSTRUMENT ID :CV1

Method: 7470A		Operator: Admin		Date of Analysis: 20 Jan 2020 15:54:03					
Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	186	-	0.0000	7470A	PPB	20 Jan 2020 15:55:25	S	Std
0.2 - 1	50.2	1004	-	0.2000	7470A	PPB	20 Jan 2020 15:57:33	S	Std
2.5 - 1	52.5	10540	-	2.5000	7470A	PPB	20 Jan 2020 15:59:40	S	Std
5.0 - 1	55.0	20753	-	5.0000	7470A	PPB	20 Jan 2020 16:01:48	S	Std
7.5 - 1	57.5	31706	-	7.5000	7470A	PPB	20 Jan 2020 16:03:54	S	Std
10.0 - 1	510.0	42712	-	10.0000	7470A	PPB	20 Jan 2020 16:06:00	S	Std
ICV73 - 1	ICV73	16423	3.8712	-	7470A	PPB	20 Jan 2020 16:15:42	U	SMPL
ICB73 - 1	ICB73	144	0.0310	-	7470A	PPB	20 Jan 2020 16:17:47	U	SMPL
CCV74 - 1	CCV74	20763	4.8950	-	7470A	PPB	20 Jan 2020 16:19:53	U	SMPL
CCB74 - 1	CCB74	147	0.0317	-	7470A	PPB	20 Jan 2020 16:21:58	U	SMPL
CRA - 1	CRA	1014	0.2362	-	7470A	PPB	20 Jan 2020 16:24:04	U	SMPL
HighStd - 1	HighStd	42163	9.9433	-	7470A	PPB	20 Jan 2020 16:26:10	U	SMPL
ChkStd - 1	ChkStd	29387	6.9294	-	7470A	PPB	20 Jan 2020 16:28:16	U	SMPL
PB126186BL - 1	PB126186BL	150	0.0324	-	7470A	PPB	20 Jan 2020 16:30:25	U	SMPL
PB126186BS - 1	PB126186BS	16340	3.8516	-	7470A	PPB	20 Jan 2020 16:32:31	U	SMPL
L1004-12 - 1	BU-02-101720	218	0.0484	-	7470A	PPB	20 Jan 2020 16:34:38	U	SMPL
L1004-12DUP - 1	BU-02-101720DUP	229	0.0510	-	7470A	PPB	20 Jan 2020 16:36:45	U	SMPL
L1004-12MS - 1	BU-02-101720MS	20458	4.8231	-	7470A	PPB	20 Jan 2020 16:38:52	U	SMPL
L1004-12MSD - 1	BU-02-101720MSD	20879	4.9224	-	7470A	PPB	20 Jan 2020 16:41:00	U	SMPL
L1014-10 - 1	OR-02-011720	204	0.0451	-	7470A	PPB	20 Jan 2020 16:43:06	U	SMPL
CCV75 - 1	CCV75	20664	4.8716	-	7470A	PPB	20 Jan 2020 16:45:12	U	SMPL
CCB75 - 1	CCB75	155	0.0336	-	7470A	PPB	20 Jan 2020 16:47:19	U	SMPL
L1166-02 - 1	QVD-WC-S-SB-BC	250	0.0560	-	7470A	PPB	20 Jan 2020 16:49:25	U	SMPL
L1166-03 - 1	QVD-WC-S-SB-01	245	0.0548	-	7470A	PPB	20 Jan 2020 16:51:30	U	SMPL
L1166-04 - 1	QVD-WC-S-SB-0203	213	0.0473	-	7470A	PPB	20 Jan 2020 16:53:36	U	SMPL
L1175-01 - 1	5-SAR-001-003-01	217	0.0482	-	7470A	PPB	20 Jan 2020 16:55:43	U	SMPL
L1181-06 - 1	930AK-AVE-COMP	238	0.0532	-	7470A	PPB	20 Jan 2020 16:57:49	U	SMPL
L1188-02 - 1	B2-0-15	201	0.0444	-	7470A	PPB	20 Jan 2020 16:59:56	U	SMPL
L1188-04 - 1	B2-15-30	200	0.0442	-	7470A	PPB	20 Jan 2020 17:02:03	U	SMPL
PB126181BL - 1	PBS	180	0.0395	-	7470A	PPB	20 Jan 2020 17:04:11	U	SMPL
PB126181BS - 1	LCSS	16198	3.8181	-	7470A	PPB	20 Jan 2020 17:06:18	U	SMPL
L1008-14 - 1	CL-01-011620	138	0.0296	-	7470A	PPB	20 Jan 2020 17:08:24	U	SMPL
CCV76 - 1	CCV76	20554	4.8457	-	7470A	PPB	20 Jan 2020 17:10:31	U	SMPL
CCB76 - 1	CCB76	142	0.0305	-	7470A	PPB	20 Jan 2020 17:12:37	U	SMPL
L1010-09 - 1	OK-02-011620	137	0.0293	-	7470A	PPB	20 Jan 2020 17:14:44	U	SMPL
L1010-09DUP - 1	OK-02-011620DUP	146	0.0315	-	7470A	PPB	20 Jan 2020 17:16:50	U	SMPL
L1010-09MS - 1	OK-02-011620MS	20210	4.7645	-	7470A	PPB	20 Jan 2020 17:18:56	U	SMPL
L1010-09MSD - 1	OK-02-011620MSD	20243	4.7723	-	7470A	PPB	20 Jan 2020 17:21:03	U	SMPL
L1012-06 - 1	EO-02-011620	109	0.0227	-	7470A	PPB	20 Jan 2020 17:23:10	U	SMPL
PB126217BL - 1	PB126217BL	158	0.0343	-	7470A	PPB	20 Jan 2020 17:25:17	U	SMPL
PB126217BS - 1	PB126217BS	16019	3.7759	-	7470A	PPB	20 Jan 2020 17:27:24	U	SMPL
L1125-06 - 1	FEQCFB-01-14-20	212	0.0470	-	7470A	PPB	20 Jan 2020 17:29:32	U	SMPL
L1125-06DUP - 1	FEQCFB-01-14-20DUP	227	0.0506	-	7470A	PPB	20 Jan 2020 17:31:40	U	SMPL
L1125-06MS - 1	FEQCFB-01-14-20MS	20006	4.7164	-	7470A	PPB	20 Jan 2020 17:33:46	U	SMPL
CCV77 - 1	CCV77	20628	4.8632	-	7470A	PPB	20 Jan 2020 17:35:52	U	SMPL
CCB77 - 1	CCB77	162	0.0352	-	7470A	PPB	20 Jan 2020 17:37:58	U	SMPL
L1125-06MSD - 1	FEQCFB-01-14-20MSD	19957	4.7049	-	7470A	PPB	20 Jan 2020 17:40:05	U	SMPL
L1165-01 - 1	QVD-GW-01-45	220	0.0489	-	7470A	PPB	20 Jan 2020 17:42:12	U	SMPL
L1166-01 - 1	QVD-WC-L-01	224	0.0499	-	7470A	PPB	20 Jan 2020 17:44:18	U	SMPL
L1173-01 - 1	0050-DECANT-H2O-COMP-2	309	0.0699	-	7470A	PPB	20 Jan 2020 17:46:24	U	SMPL
L1173-02 - 1	0053-DECANT-H2O-COMP-5	271	0.0609	-	7470A	PPB	20 Jan 2020 17:48:31	U	SMPL
L1004-12LX5 - 1		16	0.0008	-	7470A	PPB	20 Jan 2020 17:50:38	U	SMPL
L1010-09LX5 - 1		7	-0.0013	-	7470A	PPB	20 Jan 2020 17:52:45	U	SMPL
L1125-06LX5 - 1		29	0.0039	-	7470A	PPB	20 Jan 2020 17:54:53	U	SMPL
PB126181TB - 1	PB126144TB	162	0.0352	-	7470A	PPB	20 Jan 2020 17:57:00	U	SMPL
PB126186TB - 1	PB126172TB	162	0.0352	-	7470A	PPB	20 Jan 2020 17:59:07	U	SMPL
CCV78 - 1	CCV78	20416	4.8131	-	7470A	PPB	20 Jan 2020 18:01:13	U	SMPL
CCB78 - 1	CCB78	127	0.0270	-	7470A	PPB	20 Jan 2020 18:03:19	U	SMPL