

LB10744

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AK

Instrument ID : Konelab

1/29/2020 16:50

Test: Phenolics-

Sample Id	Result ^{mg/L}	Dil. 1 +	Response	Errors
ICV1	1.059	0.0	0.119	
ICB1	0.004	0.0	0.008	
CCV1	1.056	0.0	0.119	
CCB1	0.006	0.0	0.009	
PB126307BL	0.003	0.0	0.008	
PB126307BS	1.058	0.0	0.119	
L1161-10	0.030	0.0	0.011	
L1161-11	0.056	0.0	0.014	
L1233-01	0.011	0.0	0.009	
L1233-01DUP	0.011	0.0	0.009	
L1233-01MS	1.047	0.0	0.118	
L1233-01MSD	1.010	0.0	0.114	
L1256-01	0.715	0.0	0.083	
CCV2	1.053	0.0	0.118	
CCB2	0.006	0.0	0.009	

N	15
Mean	0.475
SD	0.5149
CV%	108.42

AR

Aquakem v. 7.2AQ1

Results from time period:

Wed Jan 29 15:37:36 2020

Wed Jan 29 16:48:21 2020

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0546	mg/l	1/29/2020 15:37:36	
0.1PPM	A	Phenolics-	P	0.1043	mg/l	1/29/2020 15:37:37	
0.25PPM	A	Phenolics-	P	0.2493	mg/l	1/29/2020 15:37:38	
0.50PPM	A	Phenolics-	P	0.5085	mg/l	1/29/2020 15:37:39	
1.0PPM	A	Phenolics-	P	0.9712	mg/l	1/29/2020 15:37:40	
2.0PPM	A	Phenolics-	P	2.012	mg/l	1/29/2020 15:37:41	
ICV1	S	Phenolics-	P	1.059	mg/l	1/29/2020 16:16:07	
ICB1	S	Phenolics-	P	0.0035	mg/l	1/29/2020 16:16:08	
CCV1	S	Phenolics-	P	1.0556	mg/l	1/29/2020 16:16:09	
CCB1	S	Phenolics-	P	0.006	mg/l	1/29/2020 16:16:10	
PB126307BL	S	Phenolics-	P	0.0028	mg/l	1/29/2020 16:16:11	
PB126307BS	S	Phenolics-	P	1.0583	mg/l	1/29/2020 16:16:12	
L1161-10	S	Phenolics-	P	0.0297	mg/l	1/29/2020 16:16:13	
L1161-11	S	Phenolics-	P	0.0561	mg/l	1/29/2020 16:16:14	
L1233-01	S	Phenolics-	P	0.011	mg/l	1/29/2020 16:16:15	
L1233-01DUP	S	Phenolics-	P	0.0111	mg/l	1/29/2020 16:16:16	
L1233-01MS	S	Phenolics-	P	1.0474	mg/l	1/29/2020 16:16:17	
L1233-01MSD	S	Phenolics-	P	1.0095	mg/l	1/29/2020 16:16:18	
L1256-01	S	Phenolics-	P	0.7149	mg/l	1/29/2020 16:48:19	
CCV2	S	Phenolics-	P	1.053	mg/l	1/29/2020 16:48:20	
CCB2	S	Phenolics-	P	0.0064	mg/l	1/29/2020 16:48:21	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

Instrument ID : Konelab

1/29/2020 15:47


Test Phenolics-

Accepted 1/29/2020 15:47

Factor 9.55
Bias 0.008

Coeff. of det. 0.999611

Errors

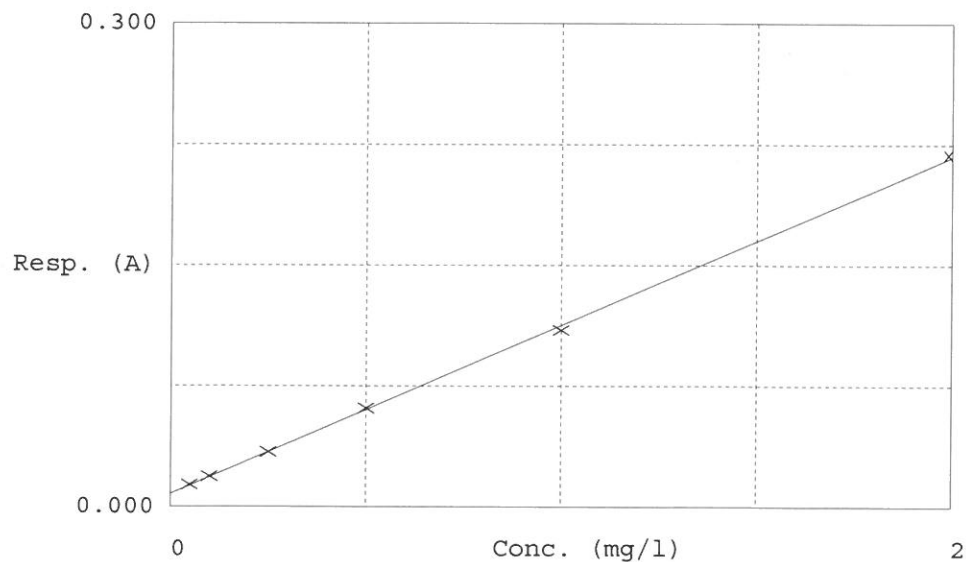

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.014	0.0546	0.0500	
2	Phenol-2	0.019	0.1043	0.1000	
3	Phenol-2	0.034	0.2493	0.2500	
4	Phenol-2	0.061	0.5085	0.5000	
5	Phenol-2	0.110	0.9712	1.0000	
6	Phenol-2	0.219	2.0120	2.0000	