

LB107566

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AK

Instrument ID : Konelab

2/5/2020 14:06

Test: Phenolics-

mg/L

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.980	0.0	0.116	
ICB1	0.007	0.0	0.009	
CCV1	0.978	0.0	0.115	
CCB1	0.007	0.0	0.009	
PB126592BS	1.001	0.0	0.118	
L1161-12	0.028	0.0	0.012	
L1377-01	0.004	0.0	0.009	
L1377-01DUP	0.004	0.0	0.009	
L1377-02MS	0.920	0.0	0.109	
L1377-03MSD	0.922	0.0	0.109	
L1377-04	0.010	0.0	0.010	
L1377-05	0.007	0.0	0.009	
PB126592BL	0.004	0.0	0.009	
CCV2	1.001	0.0	0.118	
CCB2	0.007	0.0	0.009	

N	15
Mean	0.392
SD	0.4864
CV%	124.03

AK

Aquakem v. 7.2AQ1

Results from time period:

Wed Feb 05 13:01:26 2020

Wed Feb 05 14:01:34 2020

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0517	mg/l	2/5/2020 13:01:26	
0.1PPM	A	Phenolics-	P	0.1055	mg/l	2/5/2020 13:01:27	
0.25PPM	A	Phenolics-	P	0.2571	mg/l	2/5/2020 13:01:28	
0.50PPM	A	Phenolics-	P	0.5028	mg/l	2/5/2020 13:01:29	
1.0PPM	A	Phenolics-	P	0.9696	mg/l	2/5/2020 13:01:30	
2.0PPM	A	Phenolics-	P	2.0133	mg/l	2/5/2020 13:01:31	
ICV1	S	Phenolics-	P	0.9798	mg/l	2/5/2020 13:37:23	
ICB1	S	Phenolics-	P	0.0071	mg/l	2/5/2020 13:37:24	
CCV1	S	Phenolics-	P	0.978	mg/l	2/5/2020 13:37:25	
CCB1	S	Phenolics-	P	0.0072	mg/l	2/5/2020 13:37:26	
PB126592BS	S	Phenolics-	P	1.0015	mg/l	2/5/2020 13:37:28	
L1161-12	S	Phenolics-	P	0.0284	mg/l	2/5/2020 13:37:30	
L1377-01	S	Phenolics-	P	0.0044	mg/l	2/5/2020 13:37:31	
L1377-01DUP	S	Phenolics-	P	0.0044	mg/l	2/5/2020 13:37:32	
L1377-02MS	S	Phenolics-	P	0.9202	mg/l	2/5/2020 13:37:33	
L1377-03MSD	S	Phenolics-	P	0.9215	mg/l	2/5/2020 13:37:34	
L1377-04	S	Phenolics-	P	0.0101	mg/l	2/5/2020 13:42:17	
L1377-05	S	Phenolics-	P	0.0072	mg/l	2/5/2020 13:42:18	
PB126592BL	S	Phenolics-	P	0.0042	mg/l	2/5/2020 14:01:32	
CCV2	S	Phenolics-	P	1.0008	mg/l	2/5/2020 14:01:33	
CCB2	S	Phenolics-	P	0.0073	mg/l	2/5/2020 14:01:34	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

Instrument ID : Konelab

2/5/2020 13:10

Test Phenolics-


Accepted 2/5/2020 13:10

Factor 9.164

Bias 0.009

Coeff. of det. 0.999573

Errors

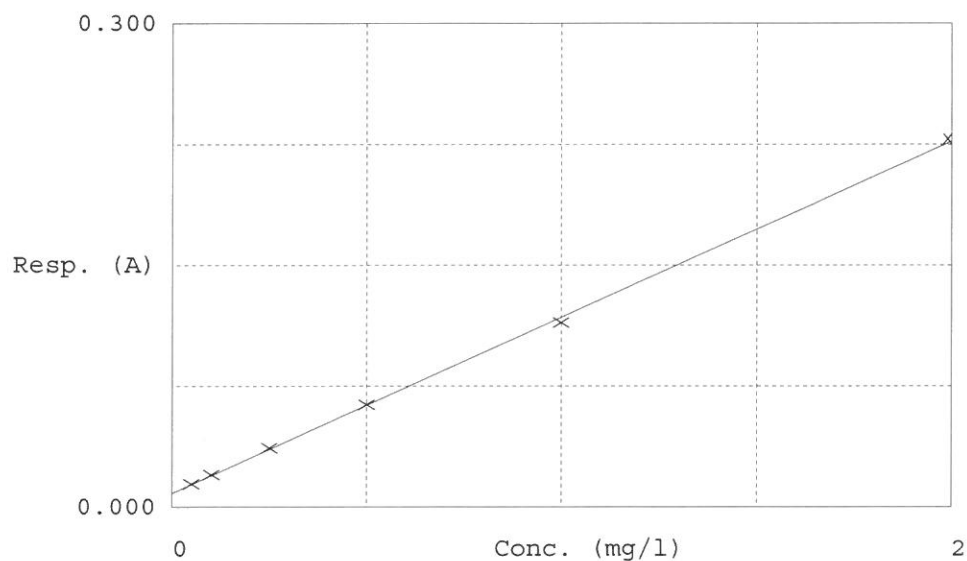

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.014	0.0517	0.0500	
2	Phenol-2	0.020	0.1055	0.1000	
3	Phenol-2	0.037	0.2571	0.2500	
4	Phenol-2	0.064	0.5028	0.5000	
5	Phenol-2	0.114	0.9696	1.0000	
6	Phenol-2	0.228	2.0133	2.0000	