

UB107702

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AR

Instrument ID : Konelab

2/11/2020 15:23

Test: ~~Total~~ ^{Reactive} CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.109	0.0	0.095	
ICB1	0.520	0.0	0.003	
CCV1	240.600	0.0	0.237	
CCB1	0.276	0.0	0.002	
PB126742BL	0.132	0.0	0.002	
L1367-04	0.178	0.0	0.002	
L1367-04DUP	0.173	0.0	0.002	
L1372-05	0.288	0.0	0.002	
L1373-03	0.217	0.0	0.002	
L1456-05	0.163	0.0	0.002	
L1475-09	0.320	0.0	0.003	
PB126744BL	0.139	0.0	0.002	
L1456-02	-0.002	0.0	0.002	
L1456-02DUP	0.013	0.0	0.002	
CCV2	253.715	0.0	0.250	
CCB2	0.296	0.0	0.002	

N	16
Mean	37.008
SD	85.3978
CV%	230.75

Aquakem v. 7.2AQ1

AK

Results from time period:

Tue Feb 11 14:58:02 2020

Tue Feb 11 15:19:33 2020

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive	Cl P	0.2516	µg/l	2/11/2020 13:06:22	
5.OPPBCN	A	Reactive	Cl P	5.1324	µg/l	2/11/2020 13:06:23	
10PPBCN	A	Reactive	Cl P	9.9566	µg/l	2/11/2020 13:06:24	
50PPBCN	A	Reactive	Cl P	49.5137	µg/l	2/11/2020 13:06:25	
100PPBCN	A	Reactive	Cl P	100.5667	µg/l	2/11/2020 13:06:26	
250PPBCN	A	Reactive	Cl P	249.2882	µg/l	2/11/2020 13:06:27	
500PPBCN	A	Reactive	Cl P	500.2907	µg/l	2/11/2020 13:06:28	
ICV1	S	Reactive	Cl P	95.1085	µg/l	2/11/2020 14:58:02	
ICB1	S	Reactive	Cl P	0.5195	µg/l	2/11/2020 14:58:03	
CCV1	S	Reactive	Cl P	240.5997	µg/l	2/11/2020 14:58:04	
CCB1	S	Reactive	Cl P	0.2765	µg/l	2/11/2020 14:58:05	
PB126742BL	S	Reactive	Cl P	0.1315	µg/l	2/11/2020 14:58:06	
L1367-04	S	Reactive	Cl P	0.178	µg/l	2/11/2020 14:58:07	
L1367-04DUP	S	Reactive	Cl P	0.1726	µg/l	2/11/2020 14:58:08	
L1372-05	S	Reactive	Cl P	0.2879	µg/l	2/11/2020 14:58:09	
L1373-03	S	Reactive	Cl P	0.2173	µg/l	2/11/2020 14:58:10	
L1456-05	S	Reactive	Cl P	0.163	µg/l	2/11/2020 14:58:11	
L1475-09	S	Reactive	Cl P	0.3204	µg/l	2/11/2020 14:58:12	
PB126744BL	S	Reactive	Cl P	0.1387	µg/l	2/11/2020 15:02:49	
L1456-02	S	Reactive	Cl P	-0.0016	µg/l	2/11/2020 15:19:30	
L1456-02DUP	S	Reactive	Cl P	0.0129	µg/l	2/11/2020 15:19:31	
CCV2	S	Reactive	Cl P	253.7147	µg/l	2/11/2020 15:19:32	
CCB2	S	Reactive	Cl P	0.2956	µg/l	2/11/2020 15:19:33	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AV

Instrument ID : Konelab

2/11/2020 13:11


Test Total CN

Accepted 2/11/2020 13:11

Factor 1025
Bias 0.002

Coeff. of det. 0.999994

Errors

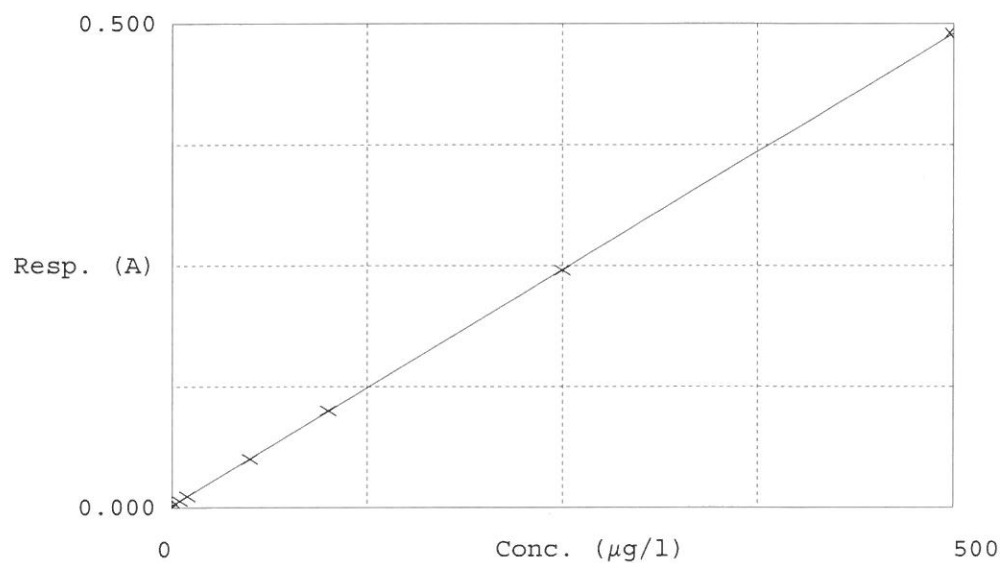

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	0.2516	0.0000	
2	5.0PPBCN	0.007	5.1324	5.0000	
3	10PPBCN	0.012	9.9566	10.0000	
4	50PPBCN	0.051	49.5137	50.0000	
5	100PPBCN	0.100	100.5667	100.0000	
6	250PPBCN	0.245	249.2882	250.0000	
7	500PPBCN	0.490	500.2907	500.0000	