

LB107814

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : Dk

Instrument ID : Konelab

2/18/2020 13:34

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.667	0.0	0.096	
ICB1	0.572	0.0	0.003	
CCV1	240.938	0.0	0.235	
CCB1	0.095	0.0	0.003	
PB126896BS	98.437	0.0	0.098	
MIDPB126896	243.333	0.0	0.237	
L1563-01	2.698	0.0	0.005	
L1563-01DUP	2.793	0.0	0.005	
L1563-01MS	8.420	0.0	0.011	
L1563-01MSD	8.596	0.0	0.011	
PB126896BL	-0.136	0.0	0.003	
CCV2	251.975	0.0	0.245	
CCB2	0.040	0.0	0.003	

N	13
Mean	73.417
SD	104.0338
CV%	141.70

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : DL

Instrument ID : Konelab

2/18/2020 10:42


Test Total CN

Accepted 2/18/2020 10:42

Factor 1038
Bias 0.003

Coeff. of det. 0.999993

Errors

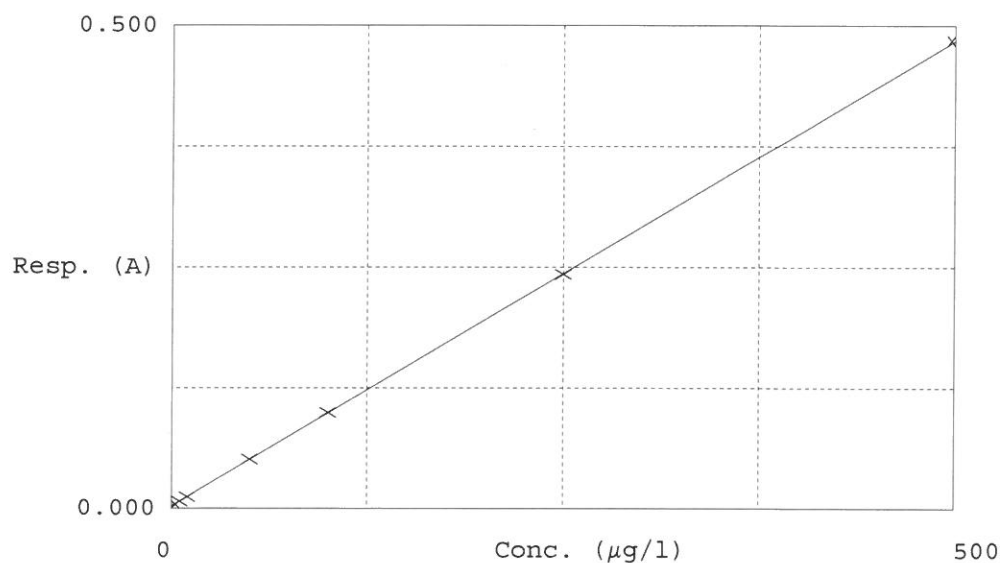

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-0.0948	0.0000	
2	5.0PPBCN	0.008	4.9822	5.0000	
3	10PPBCN	0.012	9.6339	10.0000	
4	50PPBCN	0.051	50.3520	50.0000	
5	100PPBCN	0.100	100.6708	100.0000	
6	250PPBCN	0.243	249.2355	250.0000	
7	500PPBCN	0.485	500.2204	500.0000	

Dk

Aquakem v. 7.2AQ1

Results from time period:

Tue Feb 18 10:33:14 2020

Tue Feb 18 13:33:04 2020

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	-0.0948	µg/l	2/18/2020 10:33:14	
5.0PPBCN	A	Total CN	P	4.9822	µg/l	2/18/2020 10:33:15	
10PPBCN	A	Total CN	P	9.6339	µg/l	2/18/2020 10:33:16	
50PPBCN	A	Total CN	P	50.352	µg/l	2/18/2020 10:33:17	
100PPBCN	A	Total CN	P	100.6708	µg/l	2/18/2020 10:33:18	
250PPBCN	A	Total CN	P	249.2355	µg/l	2/18/2020 10:33:19	
500PPBCN	A	Total CN	P	500.2204	µg/l	2/18/2020 10:33:20	
ICV1	S	Total CN	P	96.6666	µg/l	2/18/2020 12:53:22	
ICB1	S	Total CN	P	0.572	µg/l	2/18/2020 12:53:23	
CCV1	S	Total CN	P	240.9384	µg/l	2/18/2020 12:53:24	
CCB1	S	Total CN	P	0.0949	µg/l	2/18/2020 12:53:25	
PB126896E	S	Total CN	P	98.4367	µg/l	2/18/2020 12:53:27	
MIDPB126E	S	Total CN	P	243.333	µg/l	2/18/2020 12:53:28	
L1563-01	S	Total CN	P	2.6978	µg/l	2/18/2020 12:53:29	
L1563-01D	S	Total CN	P	2.7929	µg/l	2/18/2020 12:53:30	
L1563-01M	S	Total CN	P	8.4198	µg/l	2/18/2020 12:53:31	
L1563-01N	S	Total CN	P	8.5965	µg/l	2/18/2020 12:56:45	
PB126896E	S	Total CN	P	-0.136	µg/l	2/18/2020 13:33:02	
CCV2	S	Total CN	P	251.9746	µg/l	2/18/2020 13:33:03	
CCB2	S	Total CN	P	0.0398	µg/l	2/18/2020 13:33:04	