

LB107935

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092

Reviewed by : AK

Instrument ID : Konelab

2/24/2020 15:25

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.819	0.0	0.096	
ICB1	-1.656	0.0	0.003	
CCV1	243.983	0.0	0.238	
CCB1	-1.787	0.0	0.002	
PB127042BL	-1.731	0.0	0.003	
PB127042BS	96.822	0.0	0.097	
MIDPB127042	246.403	0.0	0.241	
L1643-01	-1.199	0.0	0.003	
L1643-01DUP	-0.973	0.0	0.003	
L1643-01MS	25.946	0.0	0.029	
L1643-01MSD	25.517	0.0	0.029	
CCV2	259.374	0.0	0.253	
CCB2	-1.744	0.0	0.003	

N	13
Mean	75.752
SD	105.2033
CV%	138.88

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AV

Instrument ID : Konelab

2/24/2020 14:57


Test Total CN

Accepted 2/24/2020 14:57

Factor 1043
Bias 0.004

Coeff. of det. 0.999879

Errors

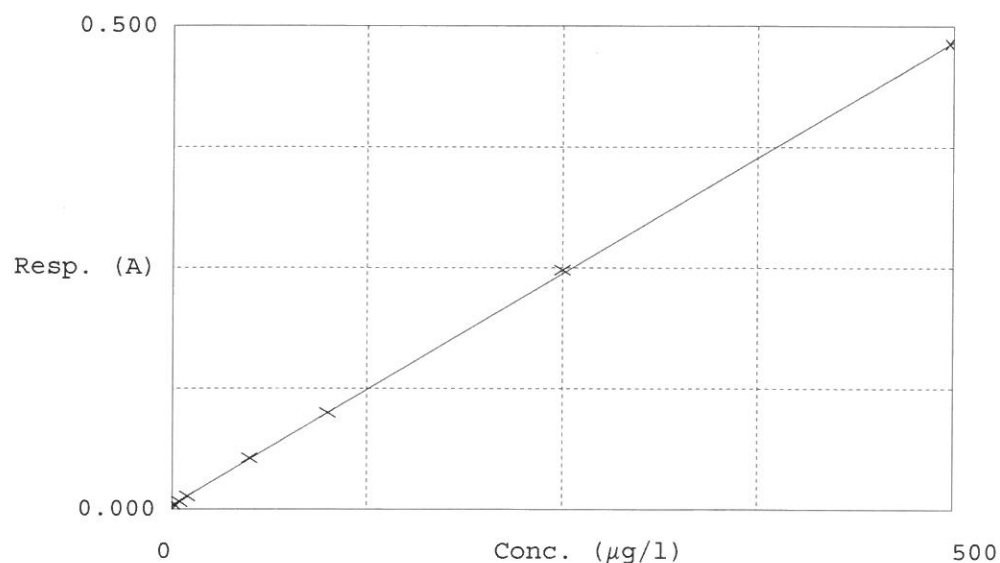

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-1.6895	0.0000	
2	5.0PPBCN	0.008	3.8717	5.0000	
3	10PPBCN	0.014	9.9950	10.0000	
4	50PPBCN	0.053	51.0360	50.0000	
5	100PPBCN	0.100	99.8939	100.0000	
6	250PPBCN	0.248	253.9279	250.0000	
7	500PPBCN	0.482	497.9651	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Mon Feb 24 14:20:39 2020

Mon Feb 24 15:25:40 2020

AC

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	-1.6895	µg/l	2/24/2020 14:56:21	
5.OPPBCN	A	Total CN	P	3.8717	µg/l	2/24/2020 14:56:22	
10PPBCN	A	Total CN	P	9.995	µg/l	2/24/2020 14:56:23	
50PPBCN	A	Total CN	P	51.036	µg/l	2/24/2020 14:56:24	
100PPBCN	A	Total CN	P	99.8939	µg/l	2/24/2020 14:56:25	
250PPBCN	A	Total CN	P	253.9279	µg/l	2/24/2020 14:56:26	
500PPBCN	A	Total CN	P	497.9651	µg/l	2/24/2020 14:56:27	
ICV1	S	Total CN	P	95.8191	µg/l	2/24/2020 15:22:16	
ICB1	S	Total CN	P	-1.6558	µg/l	2/24/2020 15:22:17	
CCV1	S	Total CN	P	243.9827	µg/l	2/24/2020 15:22:18	
CCB1	S	Total CN	P	-1.7872	µg/l	2/24/2020 15:22:19	
PB127042BL	S	Total CN	P	-1.7314	µg/l	2/24/2020 15:22:20	
PB127042BS	S	Total CN	P	96.8223	µg/l	2/24/2020 15:22:21	
MIDPB127042	S	Total CN	P	246.4029	µg/l	2/24/2020 15:22:22	
L1643-01	S	Total CN	P	-1.1988	µg/l	2/24/2020 15:22:23	
L1643-01DUP	S	Total CN	P	-0.9727	µg/l	2/24/2020 15:22:24	
L1643-01MS	S	Total CN	P	25.9457	µg/l	2/24/2020 15:22:25	
L1643-01MSD	S	Total CN	P	25.5166	µg/l	2/24/2020 15:22:26	
CCV2	S	Total CN	P	259.3738	µg/l	2/24/2020 15:25:39	
CCB2	S	Total CN	P	-1.7441	µg/l	2/24/2020 15:25:40	