

LB108528

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : DL

Instrument ID : Konelab

3/31/2020 17:33

Test: Phenolics- mg/L

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.991	0.0	0.109	
ICB1	0.003	0.0	0.004	
CCV1	1.016	0.0	0.111	
CCB1	0.001	0.0	0.004	
PB127898BL	-0.004	0.0	0.003	
PB127898BS	0.970	0.0	0.106	
L2048-02	0.005	0.0	0.004	
L2048-02DUP	0.003	0.0	0.004	
L2048-02MS	0.839	0.0	0.093	
L2048-02MSD	0.838	0.0	0.092	
CCV2	1.007	0.0	0.110	
CCB2	0.002	0.0	0.004	

N	12
Mean	0.473
SD	0.4950
CV%	104.71

Aquakem v. 7.2AQ1

Results from time period:

Tue Mar 31 16:46:09 2020

Tue Mar 31 17:29:48 2020

Dk

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.052	mg/l	3/31/2020 16:46:09	
0.1PPM	A	Phenolics-	P	0.1017	mg/l	3/31/2020 16:46:10	
0.25PPM	A	Phenolics-	P	0.2504	mg/l	3/31/2020 16:46:11	
0.50PPM	A	Phenolics-	P	0.5093	mg/l	3/31/2020 16:46:12	
1.0PPM	A	Phenolics-	P	0.9782	mg/l	3/31/2020 16:46:13	
2.0PPM	A	Phenolics-	P	2.0084	mg/l	3/31/2020 16:46:14	
ICV1	S	Phenolics-	P	0.9914	mg/l	3/31/2020 17:17:02	
ICB1	S	Phenolics-	P	0.0028	mg/l	3/31/2020 17:17:03	
CCV1	S	Phenolics-	P	1.0158	mg/l	3/31/2020 17:17:06	
CCB1	S	Phenolics-	P	0.0012	mg/l	3/31/2020 17:17:07	
PB127898BL	S	Phenolics-	P	-0.0041	mg/l	3/31/2020 17:17:10	
PB127898BS	S	Phenolics-	P	0.9704	mg/l	3/31/2020 17:17:11	
L2048-02	S	Phenolics-	P	0.0055	mg/l	3/31/2020 17:27:00	
L2048-02DUP	S	Phenolics-	P	0.0035	mg/l	3/31/2020 17:27:01	
L2048-02MS	S	Phenolics-	P	0.8394	mg/l	3/31/2020 17:27:05	
L2048-02MSD	S	Phenolics-	P	0.8378	mg/l	3/31/2020 17:27:06	
CCV2	S	Phenolics-	P	1.007	mg/l	3/31/2020 17:27:08	
CCB2	S	Phenolics-	P	0.0022	mg/l	3/31/2020 17:27:09	

LB108528

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : DL

Instrument ID : Konelab

3/31/2020 16:49


Test Phenolics-

Accepted 3/31/2020 16:49

Factor 9.456
Bias 0.004

Coeff. of det. 0.999770

Errors

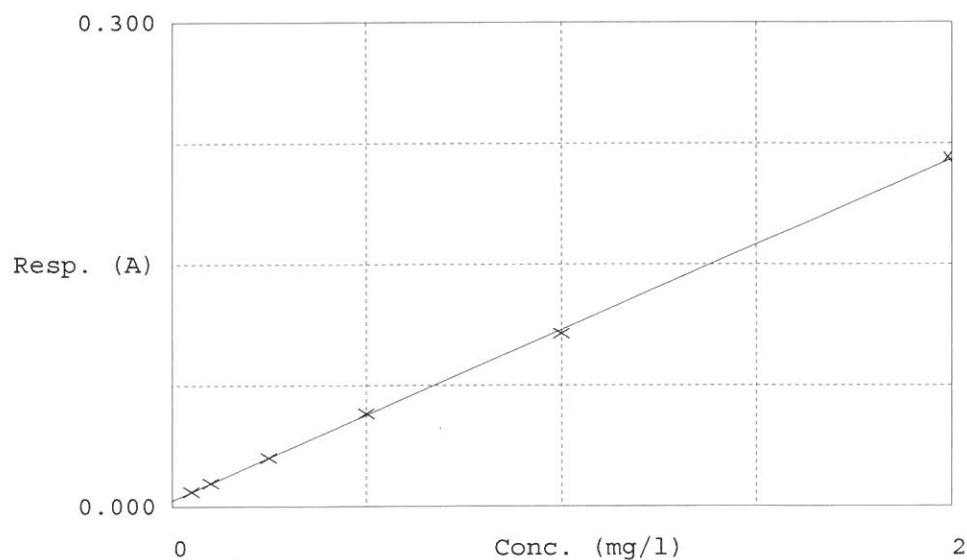

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.009	0.0520	0.0500	
2	Phenol-2	0.015	0.1017	0.1000	
3	Phenol-2	0.030	0.2504	0.2500	
4	Phenol-2	0.058	0.5093	0.5000	
5	Phenol-2	0.107	0.9782	1.0000	
6	Phenol-2	0.216	2.0084	2.0000	