

UB108583

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : Dh

Instrument ID : Konelab

4/3/2020 17:13

Test: ^{Revised} ~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.342	0.0	0.088	
ICB1	-0.982	0.0	0.002	
CCV1	241.813	0.0	0.219	
CCB1	-0.143	0.0	0.003	
PB128022BL	-0.229	0.0	0.003	
L2143-02	-0.270	0.0	0.003	
L2143-02DUP	-0.125	0.0	0.003	
PB128023BL	-0.215	0.0	0.003	
L2110-04	-0.269	0.0	0.003	
L2110-04DUP	-0.414	0.0	0.003	
L2112-06	-0.212	0.0	0.003	
L2117-05	-0.223	0.0	0.003	
L2144-01	-0.231	0.0	0.003	
L2144-02	-0.069	0.0	0.003	
CCV2	239.620	0.0	0.217	
CCB2	-0.129	0.0	0.003	
L2144-03	-0.309	0.0	0.003	
L2146-06	-0.777	0.0	0.003	
L2146-13	-0.232	0.0	0.003	
L2162-06	-0.280	0.0	0.003	
L2162-13	-0.150	0.0	0.003	
CCV3	240.984	0.0	0.218	
CCB3	-0.127	0.0	0.003	

N	23
Mean	35.321
SD	83.7647
CV%	237.15

Aquakem v. 7.2AQ1

Results from time period:

Fri Apr 03 15:36:18 2020

Fri Apr 03 16:51:09 2020

De

Sample Id	Sam/Ctr/c	Test short name	Test type	Result	Result unit	Result date and time
0.0PPBCN	A	REACTIVE CN	P	0.0703	µg/l	4/3/2020 15:36:18
5.0PPBCN	A	REACTIVE CN	P	5.2672	µg/l	4/3/2020 15:36:19
10PPBCN	A	REACTIVE CN	P	10.0836	µg/l	4/3/2020 15:36:20
50PPBCN	A	REACTIVE CN	P	49.8618	µg/l	4/3/2020 15:36:21
100PPBCN	A	REACTIVE CN	P	98.3442	µg/l	4/3/2020 15:36:22
250PPBCN	A	REACTIVE CN	P	252.0645	µg/l	4/3/2020 15:36:23
500PPBCN	A	REACTIVE CN	P	499.3084	µg/l	4/3/2020 15:36:24
ICV1	S	REACTIVE CN	P	95.342	µg/l	4/3/2020 16:35:53
ICB1	S	REACTIVE CN	P	-0.9817	µg/l	4/3/2020 16:35:54
CCV1	S	REACTIVE CN	P	241.8131	µg/l	4/3/2020 16:35:57
CCB1	S	REACTIVE CN	P	-0.1427	µg/l	4/3/2020 16:35:58
PB128022BL	S	REACTIVE CN	P	-0.2294	µg/l	4/3/2020 16:36:00
L2143-02	S	REACTIVE CN	P	-0.27	µg/l	4/3/2020 16:36:02
L2143-02DUP	S	REACTIVE CN	P	-0.125	µg/l	4/3/2020 16:43:24
PB128023BL	S	REACTIVE CN	P	-0.2151	µg/l	4/3/2020 16:43:25
L2110-04	S	REACTIVE CN	P	-0.2691	µg/l	4/3/2020 16:43:27
L2110-04DUP	S	REACTIVE CN	P	-0.4136	µg/l	4/3/2020 16:43:28
L2112-06	S	REACTIVE CN	P	-0.2116	µg/l	4/3/2020 16:43:29
L2117-05	S	REACTIVE CN	P	-0.2226	µg/l	4/3/2020 16:43:30
L2144-01	S	REACTIVE CN	P	-0.2306	µg/l	4/3/2020 16:43:31
L2144-02	S	REACTIVE CN	P	-0.0689	µg/l	4/3/2020 16:43:32
CCV2	S	REACTIVE CN	P	239.6196	µg/l	4/3/2020 16:43:34
CCB2	S	REACTIVE CN	P	-0.1292	µg/l	4/3/2020 16:50:59
L2144-03	S	REACTIVE CN	P	-0.3087	µg/l	4/3/2020 16:51:01
L2146-06	S	REACTIVE CN	P	-0.7771	µg/l	4/3/2020 16:51:02
L2146-13	S	REACTIVE CN	P	-0.2317	µg/l	4/3/2020 16:51:03
L2162-06	S	REACTIVE CN	P	-0.2799	µg/l	4/3/2020 16:51:04
L2162-13	S	REACTIVE CN	P	-0.1497	µg/l	4/3/2020 16:51:05
CCV3	S	REACTIVE CN	P	240.9844	µg/l	4/3/2020 16:51:06
CCB3	S	REACTIVE CN	P	-0.1267	µg/l	4/3/2020 16:51:09

L1408583

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : De

Instrument ID : Konelab

4/3/2020 19:02


Test ^{Pesticide} ~~Total~~ CN

Accepted 4/3/2020 15:38

Factor 1121
Bias 0.003

Coeff. of det. 0.999963

Errors

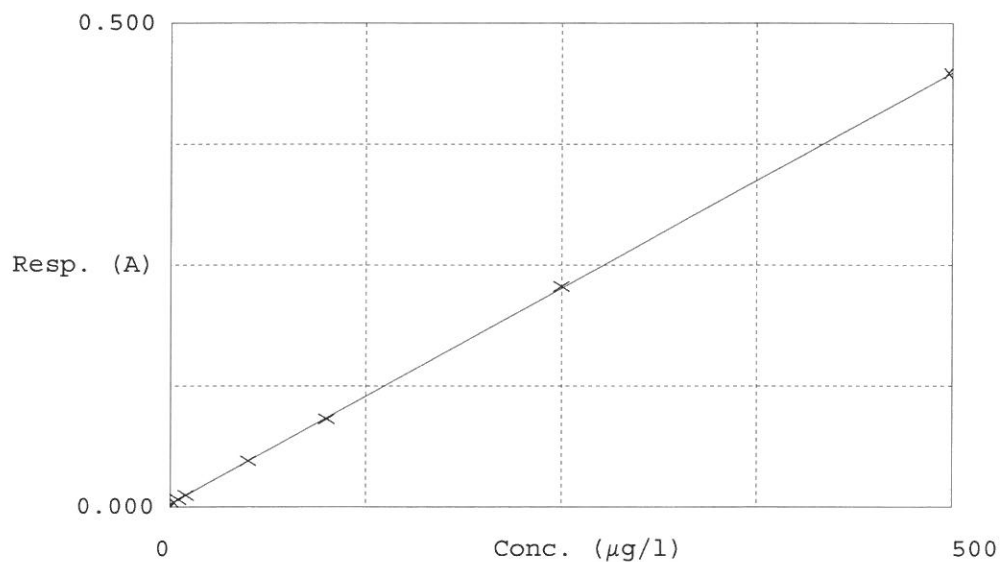

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	0.0703	0.0000	
2	5.0PPBCN	0.008	5.2672	5.0000	
3	10PPBCN	0.012	10.0836	10.0000	
4	50PPBCN	0.048	49.8618	50.0000	
5	100PPBCN	0.091	98.3442	100.0000	
6	250PPBCN	0.228	252.0645	250.0000	
7	500PPBCN	0.448	499.3084	500.0000	