

LB108665

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : DA

Instrument ID : Konelab

4/10/2020 18:02

Test: ^{Perme}
~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	98.317	0.0	0.083	
ICB1	1.554	0.0	0.003	
CCV1	244.562	0.0	0.203	
CCB1	1.647	0.0	0.004	
PB128148BL	1.405	0.0	0.003	
L2195-04	1.479	0.0	0.003	
L2195-04DUP	1.406	0.0	0.003	
L2195-08	1.474	0.0	0.003	
L2197-01	1.236	0.0	0.003	
L2197-02	1.287	0.0	0.003	
L2197-03	1.202	0.0	0.003	
L2197-04	1.344	0.0	0.003	
L2199-06	1.414	0.0	0.003	
L2199-13	1.332	0.0	0.003	
CCV2	244.990	0.0	0.204	
CCB2	1.948	0.0	0.004	
L2201-05	1.306	0.0	0.003	
L2205-08	1.325	0.0	0.003	
L2205-16	1.413	0.0	0.003	
L2205-23	1.337	0.0	0.003	
CCV3	248.589	0.0	0.207	
CCB3	1.456	0.0	0.003	

N	22
Mean	39.183
SD	86.6173
CV%	221.06

Aquakem v. 7.2AQ1

Results from time period:

Fri Apr 10 16:46:24 2020

Fri Apr 10 17:00:43 2020

1)k

Sample Id	Sam/Ctr/c/	Test short name	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	REACTIVE CN	P	0.8388	µg/l	4/10/2020 13:57:45	
5.OPPBCN	A	REACTIVE CN	P	5.7834	µg/l	4/10/2020 13:57:46	
10PPBCN	A	REACTIVE CN	P	10.7635	µg/l	4/10/2020 13:57:47	
50PPBCN	A	REACTIVE CN	P	49.8567	µg/l	4/10/2020 13:57:48	
100PPBCN	A	REACTIVE CN	P	99.1846	µg/l	4/10/2020 13:57:49	
250PPBCN	A	REACTIVE CN	P	246.8375	µg/l	4/10/2020 13:57:50	
500PPBCN	A	REACTIVE CN	P	501.7356	µg/l	4/10/2020 13:57:51	
ICV1	S	REACTIVE CN	P	98.3175	µg/l	4/10/2020 16:46:25	
ICB1	S	REACTIVE CN	P	1.5543	µg/l	4/10/2020 16:46:26	
CCV1	S	REACTIVE CN	P	244.5617	µg/l	4/10/2020 16:46:29	
CCB1	S	REACTIVE CN	P	1.6471	µg/l	4/10/2020 16:46:30	
PB128148BL	S	REACTIVE CN	P	1.4052	µg/l	4/10/2020 16:46:33	
L2195-04	S	REACTIVE CN	P	1.4793	µg/l	4/10/2020 16:46:34	
L2195-04DUP	S	REACTIVE CN	P	1.4055	µg/l	4/10/2020 16:53:56	
L2195-08	S	REACTIVE CN	P	1.4744	µg/l	4/10/2020 16:53:57	
L2197-01	S	REACTIVE CN	P	1.2365	µg/l	4/10/2020 16:53:58	
L2197-02	S	REACTIVE CN	P	1.2867	µg/l	4/10/2020 16:53:59	
L2197-03	S	REACTIVE CN	P	1.2021	µg/l	4/10/2020 16:54:00	
L2197-04	S	REACTIVE CN	P	1.3444	µg/l	4/10/2020 16:54:01	
L2199-06	S	REACTIVE CN	P	1.4136	µg/l	4/10/2020 16:54:02	
L2199-13	S	REACTIVE CN	P	1.3319	µg/l	4/10/2020 16:54:03	
CCV2	S	REACTIVE CN	P	244.99	µg/l	4/10/2020 16:54:05	
CCB2	S	REACTIVE CN	P	1.9483	µg/l	4/10/2020 16:54:06	
L2201-05	S	REACTIVE CN	P	1.3056	µg/l	4/10/2020 17:00:36	
L2205-08	S	REACTIVE CN	P	1.3248	µg/l	4/10/2020 17:00:37	
L2205-16	S	REACTIVE CN	P	1.4134	µg/l	4/10/2020 17:00:38	
L2205-23	S	REACTIVE CN	P	1.3374	µg/l	4/10/2020 17:00:39	
CCV3	S	REACTIVE CN	P	248.5894	µg/l	4/10/2020 17:00:41	
CCB3	S	REACTIVE CN	P	1.4558	µg/l	4/10/2020 17:00:42	

LB108665

=====

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by :

Instrument ID : Konelab

4/10/2020 15:56


Test ~~Total~~ CN

Accepted 4/10/2020 14:00

Factor 1216
Bias 0.002

Coeff. of det. 0.999924

Errors

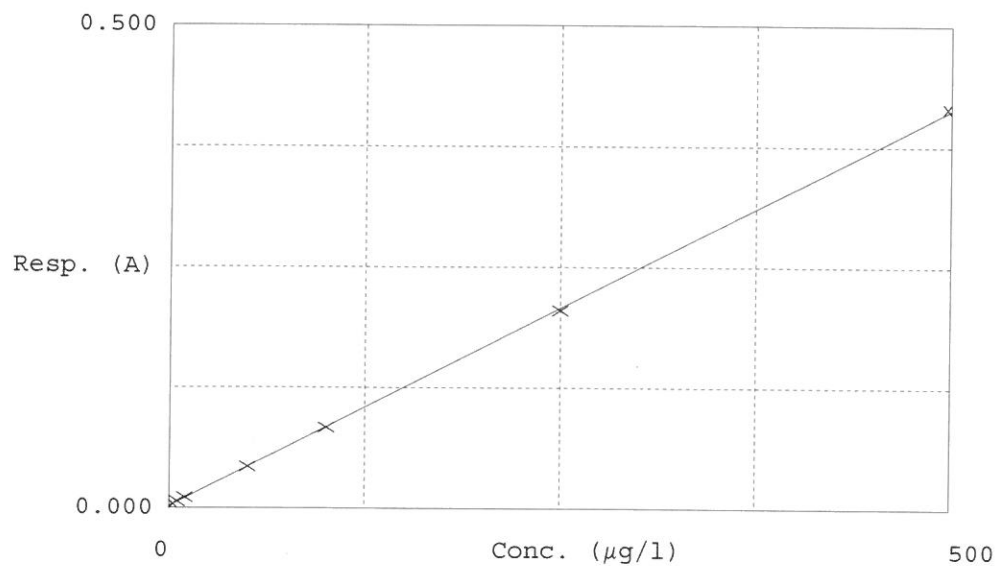

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	0.8388	0.0000	
2	5.0PPBCN	0.007	5.7834	5.0000	
3	10PPBCN	0.011	10.7635	10.0000	
4	50PPBCN	0.043	49.8567	50.0000	
5	100PPBCN	0.084	99.1846	100.0000	
6	250PPBCN	0.205	246.8375	250.0000	
7	500PPBCN	0.415	501.7356	500.0000	