

LB108723

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : Dh

Instrument ID : Konelab

4/15/2020 13:56

Test: ^{Piscine}
~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.554	0.0	0.085	
ICB1	-0.214	0.0	0.003	
CCV1	244.417	0.0	0.209	
CCB1	-0.106	0.0	0.003	
PB128239BL	-0.121	0.0	0.003	
L2123-09	0.004	0.0	0.003	
L2123-09DUP	-0.478	0.0	0.003	
L2277-04	-0.229	0.0	0.003	
L2278-01	-0.277	0.0	0.003	
L2278-02	-0.313	0.0	0.003	
L2278-03	-0.261	0.0	0.003	
L2281-11	-0.287	0.0	0.003	
L2281-14	-0.128	0.0	0.003	
CCV2	245.070	0.0	0.209	
CCB2	-0.005	0.0	0.003	

N	15
Mean	38.975
SD	87.2315
CV%	223.81

Aquakem v. 7.2AQ1

Results from time period:

Wed Apr 15 13:10:22 2020

Wed Apr 15 13:46:50 2020

DL

Sample Id	Sam/Ctr/c/	Test short name	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	REACTIVE CN	P	-0.1621	µg/l	4/15/2020 13:10:22	
5.OPPBCN	A	REACTIVE CN	P	4.5137	µg/l	4/15/2020 13:10:23	
10PPBCN	A	REACTIVE CN	P	9.3757	µg/l	4/15/2020 13:10:24	
50PPBCN	A	REACTIVE CN	P	49.3366	µg/l	4/15/2020 13:10:25	
100PPBCN	A	REACTIVE CN	P	99.738	µg/l	4/15/2020 13:10:26	
250PPBCN	A	REACTIVE CN	P	254.124	µg/l	4/15/2020 13:10:27	
500PPBCN	A	REACTIVE CN	P	498.0741	µg/l	4/15/2020 13:10:28	
ICV1	S	REACTIVE CN	P	97.5539	µg/l	4/15/2020 13:39:05	
ICB1	S	REACTIVE CN	P	-0.2142	µg/l	4/15/2020 13:39:08	
CCV1	S	REACTIVE CN	P	244.4169	µg/l	4/15/2020 13:39:10	
CCB1	S	REACTIVE CN	P	-0.1055	µg/l	4/15/2020 13:39:11	
PB128239BL	S	REACTIVE CN	P	-0.1211	µg/l	4/15/2020 13:39:13	
L2123-09	S	REACTIVE CN	P	0.0036	µg/l	4/15/2020 13:39:15	
L2123-09DUP	S	REACTIVE CN	P	-0.4781	µg/l	4/15/2020 13:46:40	
L2277-04	S	REACTIVE CN	P	-0.229	µg/l	4/15/2020 13:46:41	
L2278-01	S	REACTIVE CN	P	-0.2769	µg/l	4/15/2020 13:46:42	
L2278-02	S	REACTIVE CN	P	-0.3133	µg/l	4/15/2020 13:46:43	
L2278-03	S	REACTIVE CN	P	-0.2611	µg/l	4/15/2020 13:46:44	
L2281-11	S	REACTIVE CN	P	-0.2866	µg/l	4/15/2020 13:46:45	
L2281-14	S	REACTIVE CN	P	-0.1282	µg/l	4/15/2020 13:46:46	
CCV2	S	REACTIVE CN	P	245.0703	µg/l	4/15/2020 13:46:47	
CCB2	S	REACTIVE CN	P	-0.0052	µg/l	4/15/2020 13:46:50	

LB108723

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : DK

Instrument ID : Konelab

4/15/2020 14:02


Test ^{Perchle}
~~Total~~ CN

Accepted 4/15/2020 13:10

Factor 1190
Bias 0.003

Coeff. of det. 0.999894

Errors

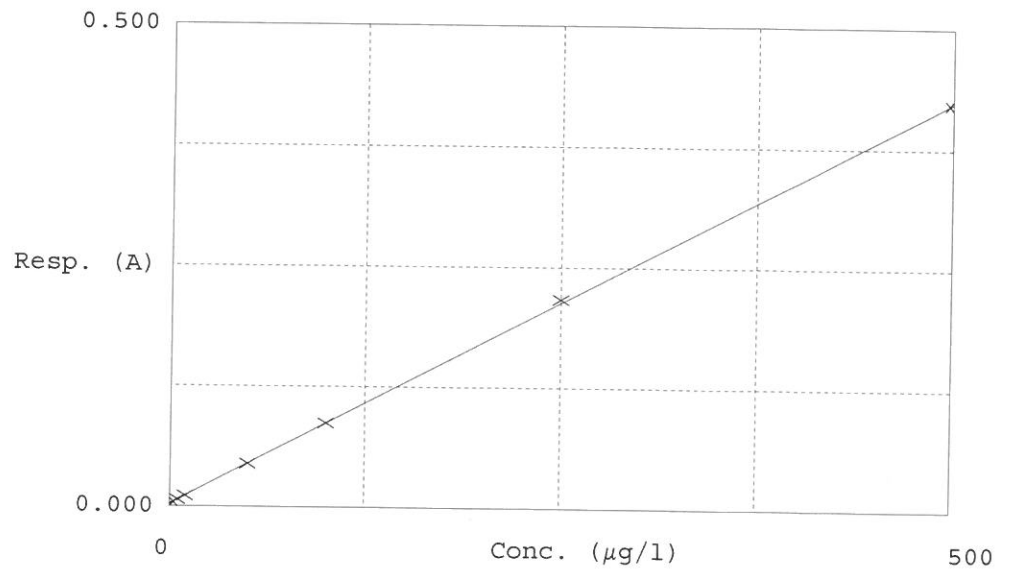

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-0.1621	0.0000	
2	5.0PPBCN	0.007	4.5137	5.0000	
3	10PPBCN	0.011	9.3757	10.0000	
4	50PPBCN	0.045	49.3366	50.0000	
5	100PPBCN	0.087	99.7380	100.0000	
6	250PPBCN	0.217	254.1240	250.0000	
7	500PPBCN	0.422	498.0741	500.0000	