

LB108800

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : DK

Instrument ID : Konelab

4/20/2020 14:50

Test: Phenolics-

mg/L

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.994	0.0	0.108	
ICB1	0.009	0.0	0.006	
CCV1	1.028	0.0	0.112	
CCB1	0.018	0.0	0.007	
PB128324BL	0.007	0.0	0.006	
PB128324BS	0.996	0.0	0.109	
L2286-01	0.008	0.0	0.006	
L2286-01DUP	0.006	0.0	0.006	
L2286-01MS	0.984	0.0	0.107	
L2286-01MSD	0.989	0.0	0.108	
CCV2	1.010	0.0	0.110	
CCB2	0.028	0.0	0.008	

N 12
Mean 0.507
SD 0.5159
CV% 101.86

Aquakem v. 7.2AQ1

Results from time period:

Mon Apr 20 13:53:27 2020

Mon Apr 20 14:45:31 2020

1/2

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0522	mg/l	4/20/2020 13:53:27	
0.1PPM	A	Phenolics-	P	0.1017	mg/l	4/20/2020 13:53:28	
0.25PPM	A	Phenolics-	P	0.2416	mg/l	4/20/2020 13:53:29	
0.50PPM	A	Phenolics-	P	0.495	mg/l	4/20/2020 13:53:30	
1.0PPM	A	Phenolics-	P	1.0147	mg/l	4/20/2020 13:53:31	
2.0PPM	A	Phenolics-	P	1.9948	mg/l	4/20/2020 13:53:32	
ICV1	S	Phenolics-	P	0.994	mg/l	4/20/2020 14:18:27	
ICB1	S	Phenolics-	P	0.0085	mg/l	4/20/2020 14:18:28	
CCV1	S	Phenolics-	P	1.0282	mg/l	4/20/2020 14:18:30	
CCB1	S	Phenolics-	P	0.018	mg/l	4/20/2020 14:18:33	
PB128324BL	S	Phenolics-	P	0.0068	mg/l	4/20/2020 14:18:35	
PB128324BS	S	Phenolics-	P	0.9963	mg/l	4/20/2020 14:18:36	
L2286-01	S	Phenolics-	P	0.0084	mg/l	4/20/2020 14:26:08	
L2286-01DUP	S	Phenolics-	P	0.0061	mg/l	4/20/2020 14:26:09	
L2286-01MS	S	Phenolics-	P	0.9841	mg/l	4/20/2020 14:26:12	
L2286-01MSD	S	Phenolics-	P	0.9889	mg/l	4/20/2020 14:26:13	
CCV2	S	Phenolics-	P	1.0104	mg/l	4/20/2020 14:26:15	
CCB2	S	Phenolics-	P	0.0283	mg/l	4/20/2020 14:45:31	

LB108800

=====

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : DA

Instrument ID : Konelab

4/20/2020 13:55

Test Phenolics-


Accepted 4/20/2020 13:55

Factor 9.634

Bias 0.005

Coeff. of det. 0.999875

Errors

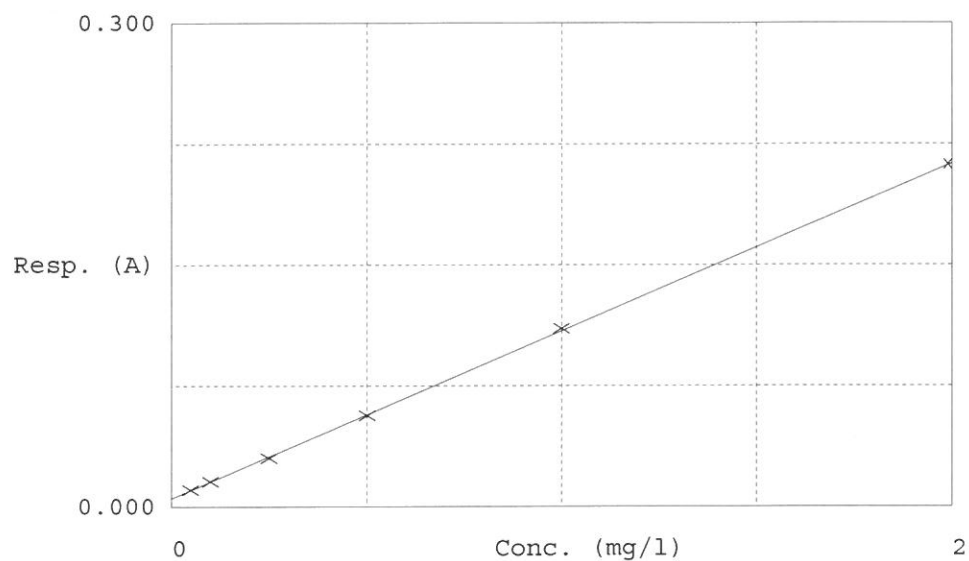

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.011	0.0522	0.0500	
2	Phenol-2	0.016	0.1017	0.1000	
3	Phenol-2	0.030	0.2416	0.2500	
4	Phenol-2	0.057	0.4950	0.5000	
5	Phenol-2	0.111	1.0147	1.0000	
6	Phenol-2	0.212	1.9948	2.0000	