

LB108819

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : *AL*

Instrument ID : Konelab

4/21/2020 14:08

Test: Total CN *my/c*

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.459	0.0	0.086	
ICB1	0.568	0.0	0.003	
CCV1	245.501	0.0	0.212	
CCB1	0.534	0.0	0.003	
PB128328BL	0.487	0.0	0.003	
PB128328BS	97.051	0.0	0.085	
MIDPB128328	245.676	0.0	0.212	
L2182-10	2.338	0.0	0.005	
L2182-11	4.393	0.0	0.006	
L2326-01	0.988	0.0	0.004	
L2326-01DUP	0.848	0.0	0.003	
L2326-01MS	25.090	0.0	0.024	
L2326-01MSD	25.222	0.0	0.024	
CCV2	247.133	0.0	0.213	
CCB2	0.681	0.0	0.003	

N	15
Mean	66.265
SD	98.5783
CV%	148.76

Aquakem v. 7.2AQ1

Results from time period:

Tue Apr 21 11:59:08 2020

Tue Apr 21 13:04:10 2020

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	0.2945	µg/l	4/21/2020 11:59:08	
5.OPPBCN	A	Total CN	P	5.1153	µg/l	4/21/2020 11:59:09	
10PPBCN	A	Total CN	P	9.6779	µg/l	4/21/2020 11:59:10	
50PPBCN	A	Total CN	P	50.2682	µg/l	4/21/2020 11:59:11	
100PPBCN	A	Total CN	P	98.2381	µg/l	4/21/2020 11:59:12	
250PPBCN	A	Total CN	P	252.1503	µg/l	4/21/2020 11:59:13	
500PPBCN	A	Total CN	P	499.2557	µg/l	4/21/2020 11:59:14	
ICV1	S	Total CN	P	97.4595	µg/l	4/21/2020 12:49:23	
ICB1	S	Total CN	P	0.5676	µg/l	4/21/2020 12:49:24	
CCV1	S	Total CN	P	245.5005	µg/l	4/21/2020 12:49:26	
CCB1	S	Total CN	P	0.5343	µg/l	4/21/2020 12:49:29	
PB128328BL	S	Total CN	P	0.4872	µg/l	4/21/2020 12:49:31	
PB128328BS	S	Total CN	P	97.0505	µg/l	4/21/2020 12:49:32	
MIDPB128328	S	Total CN	P	245.676	µg/l	4/21/2020 12:56:56	
L2182-10	S	Total CN	P	2.3378	µg/l	4/21/2020 12:56:57	
L2182-11	S	Total CN	P	4.3927	µg/l	4/21/2020 12:57:02	
L2326-01	S	Total CN	P	0.9877	µg/l	4/21/2020 13:04:01	
L2326-01DUP	S	Total CN	P	0.8481	µg/l	4/21/2020 13:04:02	
L2326-01MS	S	Total CN	P	25.0905	µg/l	4/21/2020 13:04:05	
L2326-01MSD	S	Total CN	P	25.222	µg/l	4/21/2020 13:04:06	
CCV2	S	Total CN	P	247.133	µg/l	4/21/2020 13:04:08	
CCB2	S	Total CN	P	0.6806	µg/l	4/21/2020 13:04:09	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : DH

Instrument ID : Konelab

4/21/2020 16:06


Test Total CN

Accepted 4/21/2020 12:09

Factor 1174
Bias 0.003

Coeff. of det. 0.999958

Errors

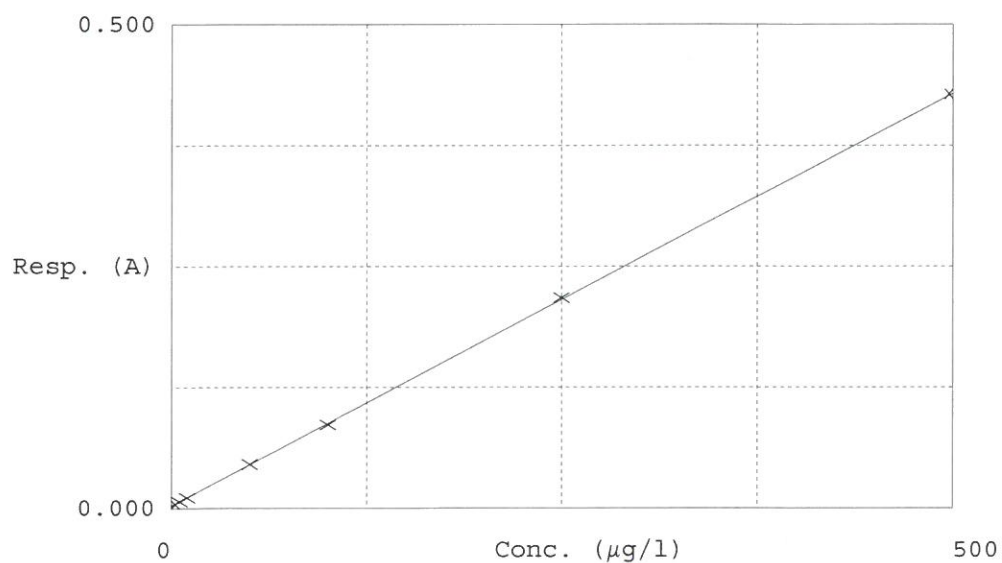

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	0.2945	0.0000	
2	5.0PPBCN	0.007	5.1153	5.0000	
3	10PPBCN	0.011	9.6779	10.0000	
4	50PPBCN	0.046	50.2682	50.0000	
5	100PPBCN	0.086	98.2381	100.0000	
6	250PPBCN	0.218	252.1503	250.0000	
7	500PPBCN	0.428	499.2557	500.0000	