

IC-2
M300.0
4/28/2020
AM


Clear table

ident	concentra tion F-	concentrati on CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2020-04-21	4/21/20 12:11		AM/AP
STD2	0.2640	0.3430	0.3820	1.1490	0.2900	0.5250	1.7760	2020-04-21	4/21/20 12:44		AM/AP
STD3	0.3930	0.6150	0.6270	2.0360	0.5050	0.9720	3.1180	2020-04-21	4/21/20 13:17		AM/AP
STD4	0.8090	1.1880	1.1740	3.9700	0.9970	1.9780	5.9120	2020-04-21	4/21/20 13:47		AM/AP
STD5	1.9140	2.9190	2.8790	9.7330	2.4290	5.0120	14.4990	2020-04-21	4/21/20 14:18		AM/AP
STD6	3.9660	6.0210	5.9730	20.0650	5.0170	10.0660	30.0570	2020-04-21	4/21/20 14:48		AM/AP
STD7	5.0550	7.5130	7.5660	25.0460	6.2620	12.4460	37.6380	2020-04-21	4/21/20 15:19		AM/AP
ICV	1.9280	2.9240	2.8700	9.7490	2.4430	5.0680	14.4950	2020-04-21	4/21/20 15:52		AM/AP
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2020-04-21	4/21/20 16:23		AM/AP
CCV	1.9220	2.8750	2.7660	9.5950	2.3720	4.8020	14.2820	2020-04-22	4/22/20 10:11		AM/AP
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2020-04-22	4/22/20 10:41		AM/AP
LB108832BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2020-04-22	4/22/20 11:12		AM/AP
LB108832BSW	1.9390	2.8740	2.7850	9.6010	2.3750	4.9180	14.2810	2020-04-22	4/22/20 11:42		AM/AP
L2384-01	0.0000	0.1900	0.0000	0.0000	0.0000	0.0000	0.0000	2020-04-22	4/22/20 13:13		AM/AP
L2384-01DUP	0.0000	0.1850	0.0000	0.0000	0.0000	0.0000	0.0000	2020-04-22	4/22/20 13:43		AM/AP
L2384-01MS	1.9550	3.0640	2.7860	9.7350	2.4420	4.6840	14.5850	2020-04-22	4/22/20 14:14		AM/AP
L2384-01MSD	1.8370	2.9370	2.6820	9.3620	2.3330	4.5470	14.0120	2020-04-22	4/22/20 14:45		AM/AP
L2182-07	0.1840	0.2030	0.2500	0.6850	0.1720	0.3440	1.1060	2020-04-22	4/22/20 15:15		AM/AP
L2182-08	0.2490	0.3400	0.3680	1.1490	0.2950	0.5390	1.7620	2020-04-22	4/22/20 15:46		AM/AP
L2182-08RE	0.3960	0.6150	0.6110	2.0590	0.5070	0.9920	3.1230	2020-04-22	4/22/20 16:16		AM/AP
CCV	1.9980	2.9020	2.7860	9.6570	2.3920	5.2160	14.3630	2020-04-22	4/22/20 16:47		AM/AP
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2020-04-22	4/22/20 17:18		AM/AP

CALIBRATION OF COMPONENT F-

Method: AnionsIC2-042120.mtw
 Equation: $Q = 0.0808174 \cdot A + 2.02171$
 RSD: 3.052 %
 Correlation coefficient: 0.999606

IC-2
 M300.0
 4/22/2020
 AM

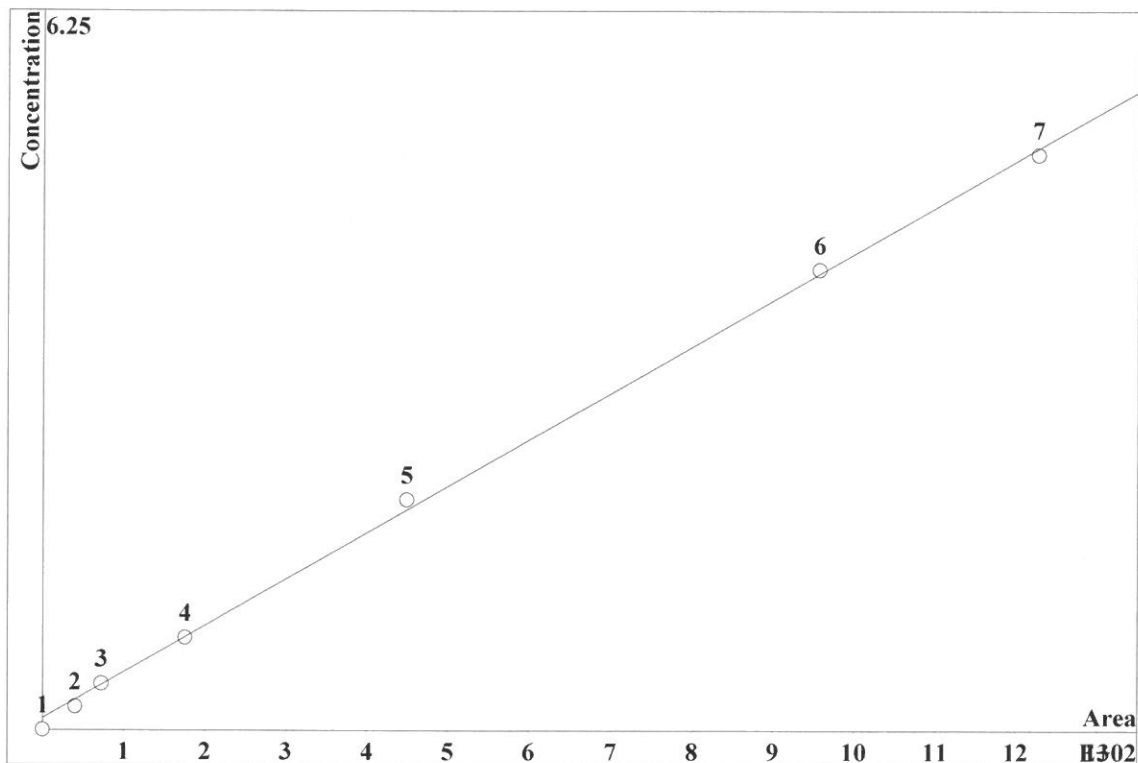


K3 = 0 K2 = 0 K1 = 0.0808174 K0 = 2.02171
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		
2	0.9378	40.25	0.2	20	5.75		
3	1.892	72.23	0.4	20	5.75		
4	4.566	175.1	0.8	20	5.75		
5	12.24	448.5	2	20	5.75		
6	27.48	956.4	4	20	5.75		
7	35.54	1226	5	20	5.75		

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-042120.mtw
 Equation: $Q = 0.125849 \cdot A + 1.52293$
 RSD: 1.559 %
 Correlation coefficient: 0.999897




K3 = 0 K2 = 0 K1 = 0.125849 K0 = 1.52293
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0		0	0			0
2	2.265	42.46	0.3	20			8.834
3	4.597	85.58	0.6	20			8.834
4	9.394	176.8	1.2	20			8.834
5	24.11	451.9	3	20			8.834
6	51.33	944.8	6	20			8.834
7	64.04	1182	7.5	20			8.834

CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-042120.mtw
 Equation: $Q = 0.056277 \cdot A + 3.06996$
 RSD: 2.699 %
 Correlation coefficient: 0.999692

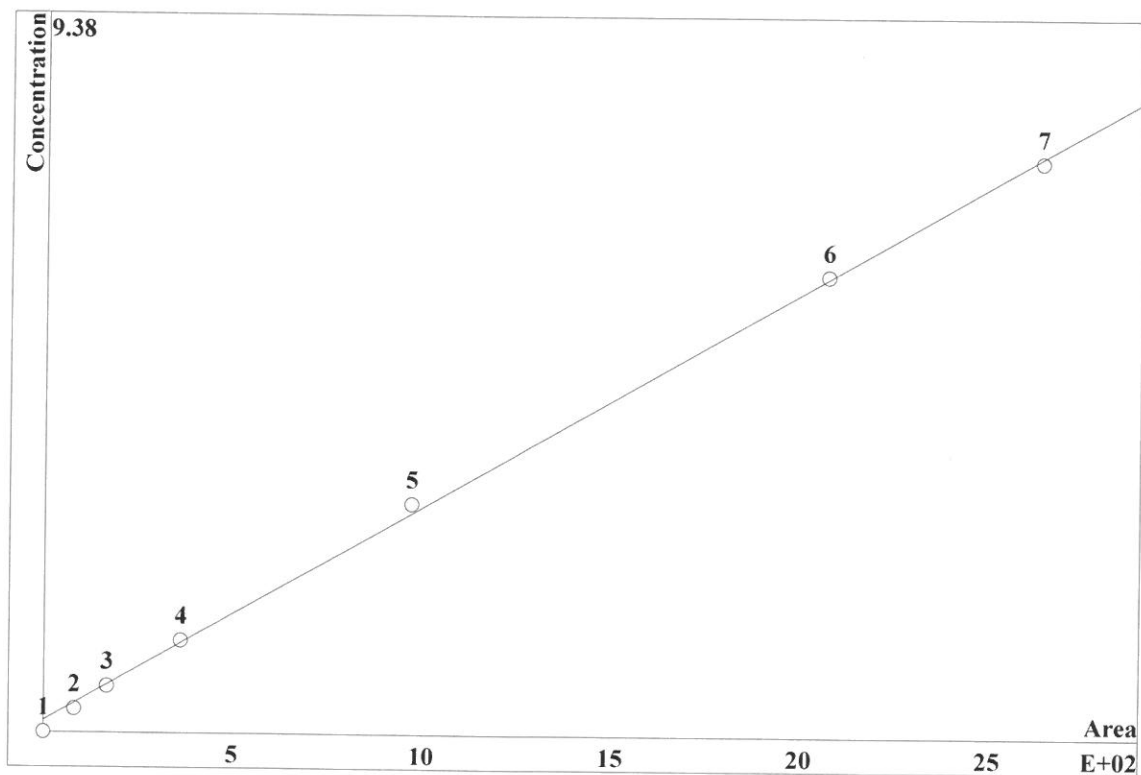


K3 = 0 K2 = 0 K1 = 0.056277 K0 = 3.06996
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1		0	0	0	0		
2	3.535	81.32	0.3	20	10.73		
3	7.093	168.4	0.6	20	10.73		
4	14.85	362.6	1.2	20	10.73		
5	37.43	968.4	3	20	10.73		
6	75.59	2068	6	20	10.73		
7	93.79	2634	7.5	20	10.73		

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-042120.mtw
 Equation: $Q = 0.283724 \cdot A + 5.37926$
 RSD: 1.545 %
 Correlation coefficient: 0.999899

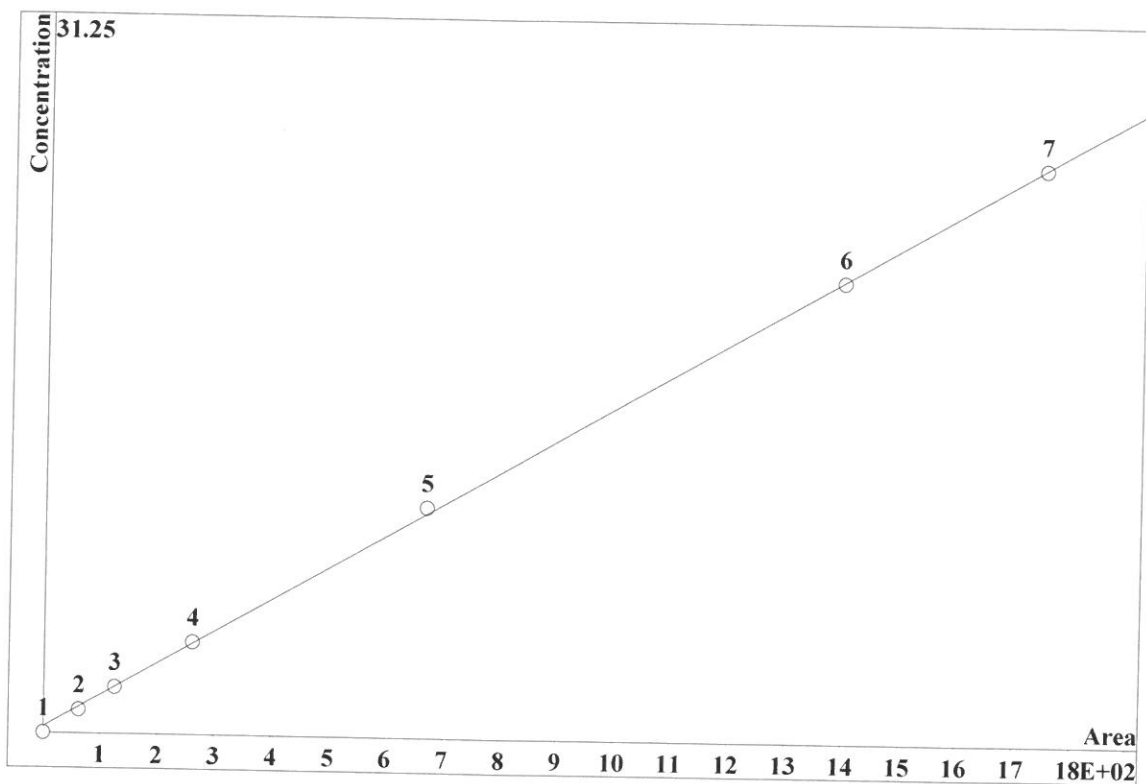


K3 = 0 K2 = 0 K1 = 0.283724 K0 = 5.37926
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	2.186	62.02	1	20			14
3	4.422	124.6	2	20			14
4	9.206	260.9	4	20			14
5	23.84	667.1	10	20			14
6	51.08	1395	20	20			14
7	64.08	1747	25	20			14

Ⓜ

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-042120.mtw
 Equation: $Q = 0.0495992 \cdot A + 1.30724$
 RSD: 1.624 %
 Correlation coefficient: 0.999889




K3 = 0 K2 = 0 K1 = 0.0495992 K0 = 1.30724
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used File
1	0	0	0	0	0	0
2	2.585	90.54	0.25	20	16.26	
3	5.234	177.3	0.5	20	16.26	
4	10.78	375.5	1	20	16.26	
5	27.09	953.3	2.5	20	16.26	
6	56.19	1997	5	20	16.26	
7	69.3	2499	6.25	20	16.26	

CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-042120.mtw
 Equation: $Q = 0.0952609 \cdot A + 3.17883$
 RSD: 0.935 %
 Correlation coefficient: 0.999963

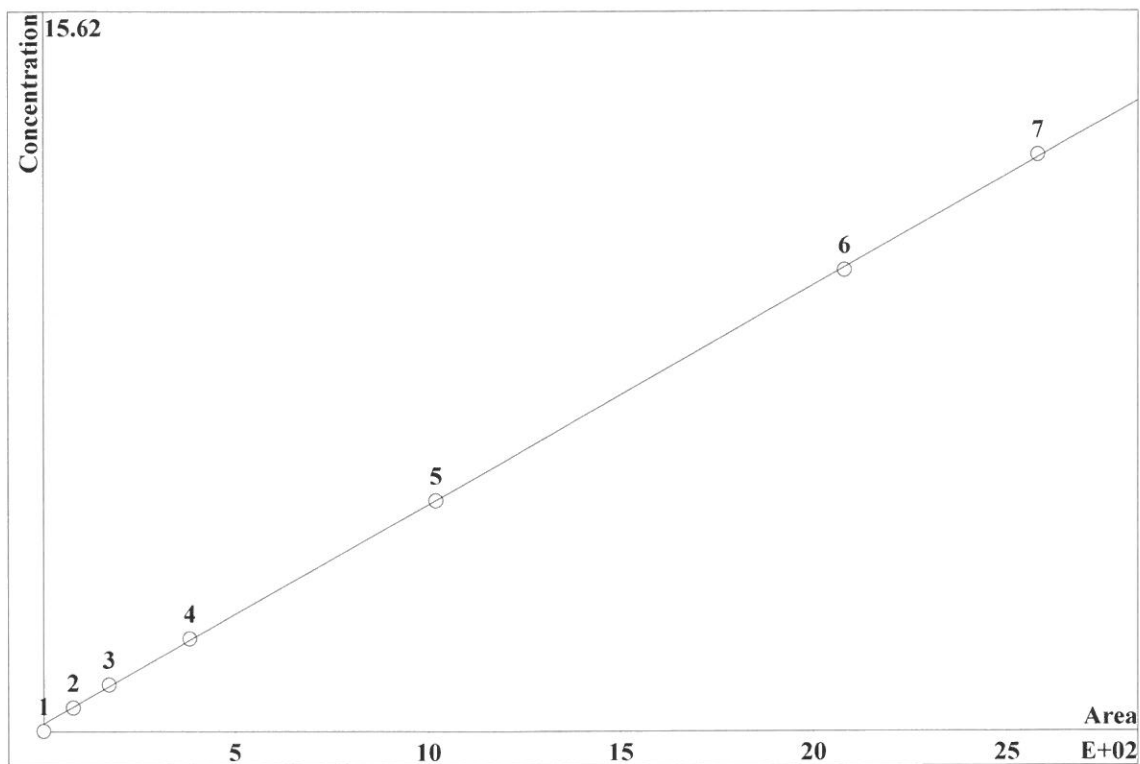


K3 = 0 K2 = 0 K1 = 0.0952609 K0 = 3.17883
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	1.682	76.89	0.5	20	21.2		
3	3.689	170.8	1	20	21.2		
4	8.063	381.9	2	20	21.2		
5	21.59	1019	5	20	21.2		
6	45.69	2080	10	20	21.2		
7	56.7	2580	12.5	20	21.2		

CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-042120.mtw
 Equation: $Q = 0.167029 \cdot A + 7.87332$
 RSD: 1.965 %
 Correlation coefficient: 0.999837

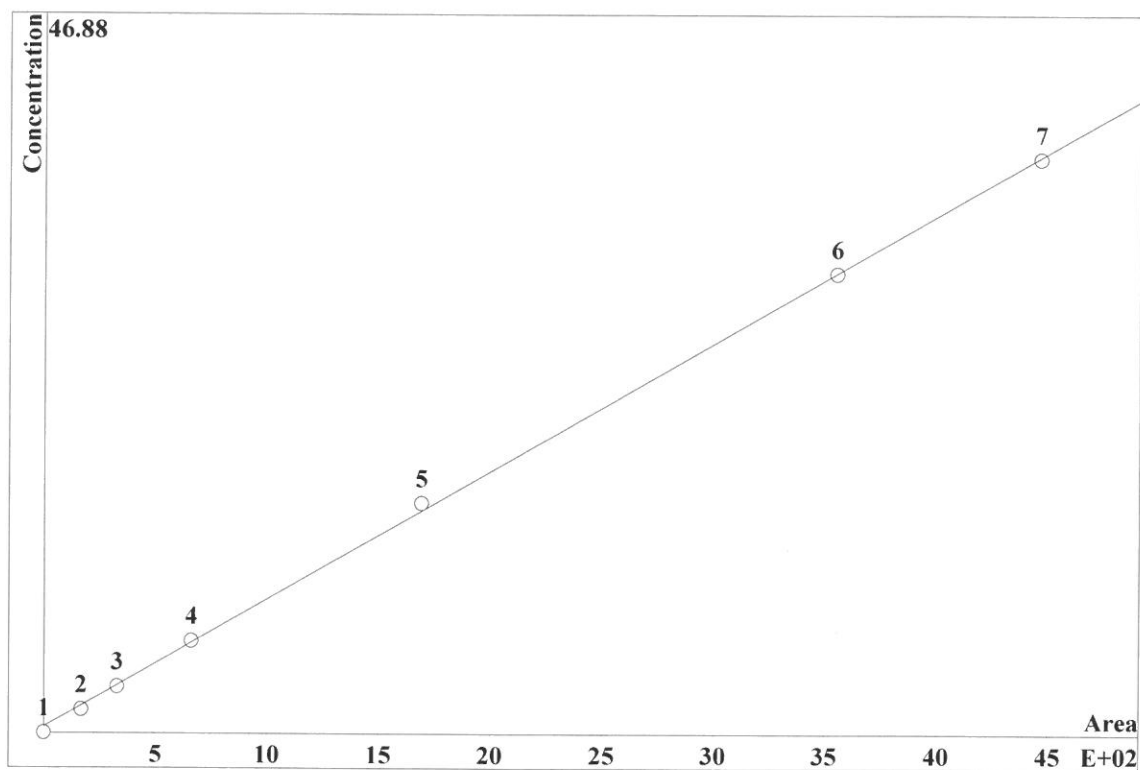

K3 = 0 K2 = 0 K1 = 0.167029 K0 = 7.87332
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	3.903	165.5	1.5	20	24.57		
3	7.715	326.2	3	20	24.57		
4	15.73	660.7	6	20	24.57		
5	40.59	1689	15	20	24.57		
6	86.75	3552	30	20	24.57		
7	108.7	4460	37.5	20	24.57		

Report date: 4/22/2020 9:12:26 AM
Printed by: wet


Ident: STD1
Analysis from: 4/21/2020 12:11:45 PM
File: _2020-04-21_

Last save: 4/22/2020 9:12:20 AM

Method: AnionsIC2-042120.mtw
Run operator: wet
Analysis number: 25075

Last save: 4/21/2020 2:26:

SAMPLE:
: AM/AP
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 4/22/2020 9:12:36 AM
Printed by: wet


Ident: STD2
Analysis from: 4/21/2020 12:44:23 PM
File: _2020-04-21_

Last save: 4/22/2020 9:12:20 AM

Method: AnionsIC2-042120.mtw
Run operator: wet
Analysis number: 25076

Last save: 4/21/2020 2:26:

SAMPLE:
: AM/AP
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.75	0.523	0.94	5.47	40.248	7.20
2	8.83	0.239	2.27	13.25	42.460	7.60
3	10.73	0.306	3.53	20.68	81.319	14.55
4	14.00	0.366	2.18	12.78	62.020	11.10
5	16.26	0.438	2.58	15.12	90.544	16.20
6	21.20	0.511	1.68	9.82	76.895	13.76
7	24.57	0.493	3.90	22.83	165.485	29.61
7	30.00	0.411	17.09	99.95	558.971	100.00

This report has been created by IC Net
METROHM LTD

Report date: 4/22/2020 9:12:44 AM
Printed by: wet


Ident: STD3
Analysis from: 4/21/2020 1:17:01 PM
File: _2020-04-21_

Last save: 4/22/2020 9:12:20 AM

Method: AnionsIC2-042120.mtw
Run operator: wet
Analysis number: 25077

Last save: 4/21/2020 2:26:

SAMPLE:
: AM/AP
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

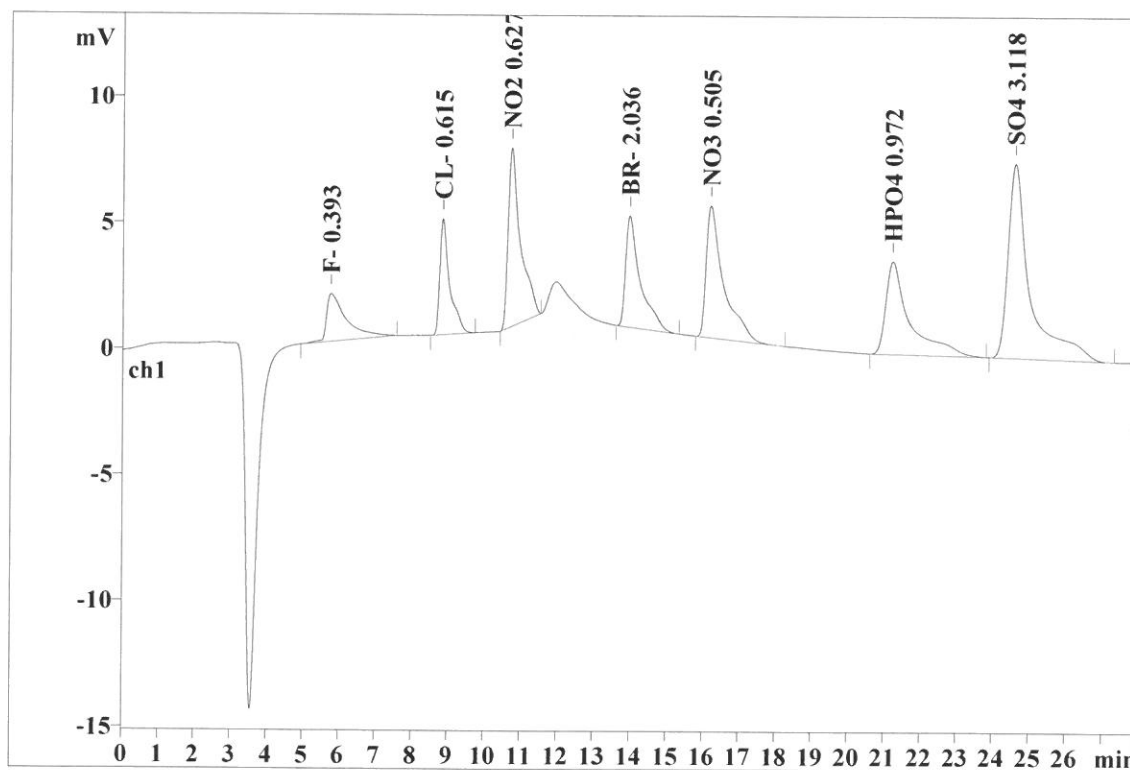

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.74	0.492	1.89	5.45	72.228	6.42
2	8.82	0.240	4.59	13.26	85.575	7.61
3	10.71	0.311	7.09	20.47	168.373	14.97
4	13.95	0.361	4.42	12.76	124.583	11.07
5	16.18	0.432	5.23	15.11	177.298	15.76
6	21.20	0.519	3.69	10.65	170.770	15.18
7	24.58	0.490	7.72	22.27	326.212	29.00
7	28.00	0.407	34.64	99.98	1125.039	100.00

This report has been created by IC Net
METROHM LTD

Report date: 4/22/2020 9:12:51 AM
Printed by: wet


Ident: STD4
Analysis from: 4/21/2020 1:47:39 PM
File: _2020-04-21_

Last save: 4/22/2020 9:12:20 AM

Method: AnionsIC2-042120.mtw
Run operator: wet
Analysis number: 25078

Last save: 4/21/2020 2:26:

SAMPLE:
: AM/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.78	0.481	4.56	6.29	175.093	7.32
2	8.85	0.241	9.39	12.94	176.758	7.39
3	10.72	0.312	14.85	20.46	362.595	15.15
4	13.94	0.360	9.21	12.68	260.890	10.90
5	16.15	0.440	10.78	14.85	375.505	15.69
6	21.30	0.528	8.06	11.11	381.883	15.96
7	24.67	0.488	15.72	21.66	660.722	27.61
7	28.00	0.407	72.58	99.99	2393.446	100.00

This report has been created by IC Net
METROHM LTD

Report date: 4/22/2020 9:12:58 AM
Printed by: wet


Ident: STD5
Analysis from: 4/21/2020 2:18:18 PM
File: _2020-04-21_

Last save: 4/22/2020 9:12:20 AM

Method: AnionsIC2-042120.mtw
Run operator: wet
Analysis number: 25079

Last save: 4/21/2020 2:26:

SAMPLE:
: AM/AP
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

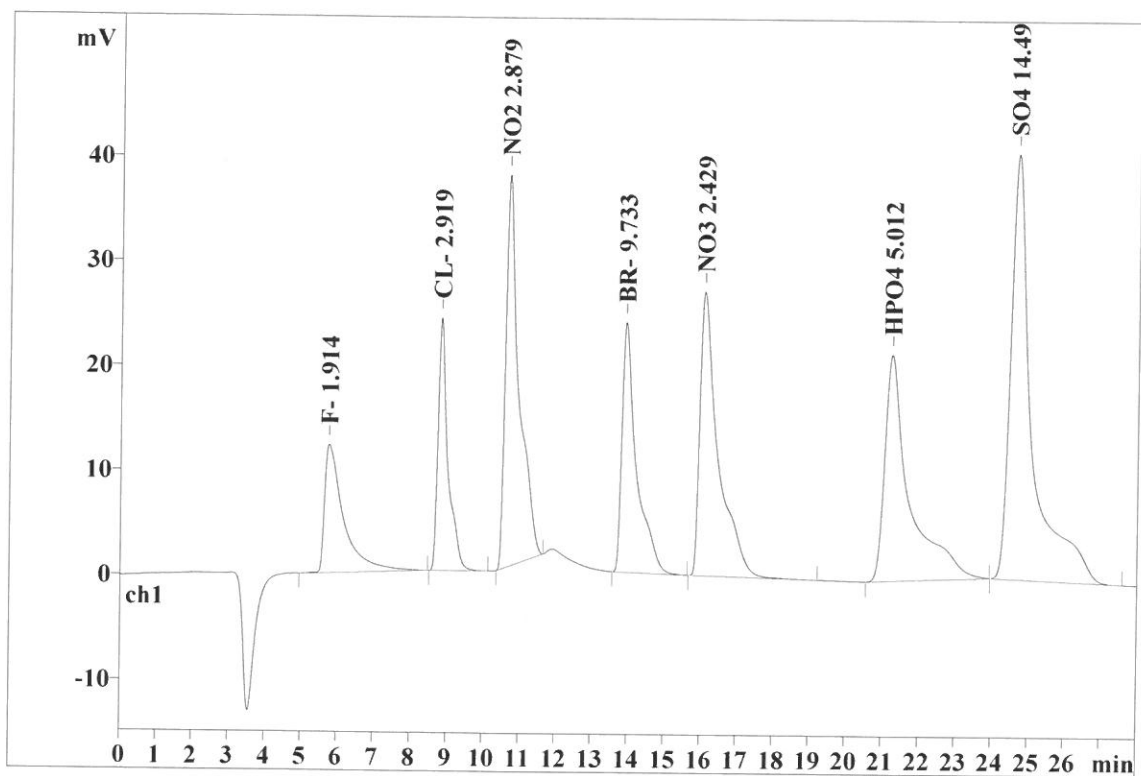

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.76	0.473	12.23	6.55	448.522	7.24
2	8.81	0.240	24.11	12.90	451.858	7.29
3	10.66	0.331	37.42	20.02	968.438	15.63
4	13.91	0.356	23.84	12.76	667.148	10.77
5	16.07	0.451	27.09	14.50	953.270	15.38
6	21.24	0.524	21.59	11.55	1018.957	16.44
7	24.66	0.483	40.59	21.72	1688.984	27.25
7	28.00	0.408	186.88	100.00	6197.176	100.00

This report has been created by IC Net
METROHM LTD

Report date: 4/22/2020 9:13:06 AM
Printed by: wet


Ident: STD6
Analysis from: 4/21/2020 2:48:56 PM
File: _2020-04-21_

Last save: 4/21/2020 3:49:40 PM

Method: AnionsIC2-042120.mtw
Run operator: wet
Analysis number: 25080

Last save: 4/21/2020 2:26:

SAMPLE:
:
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

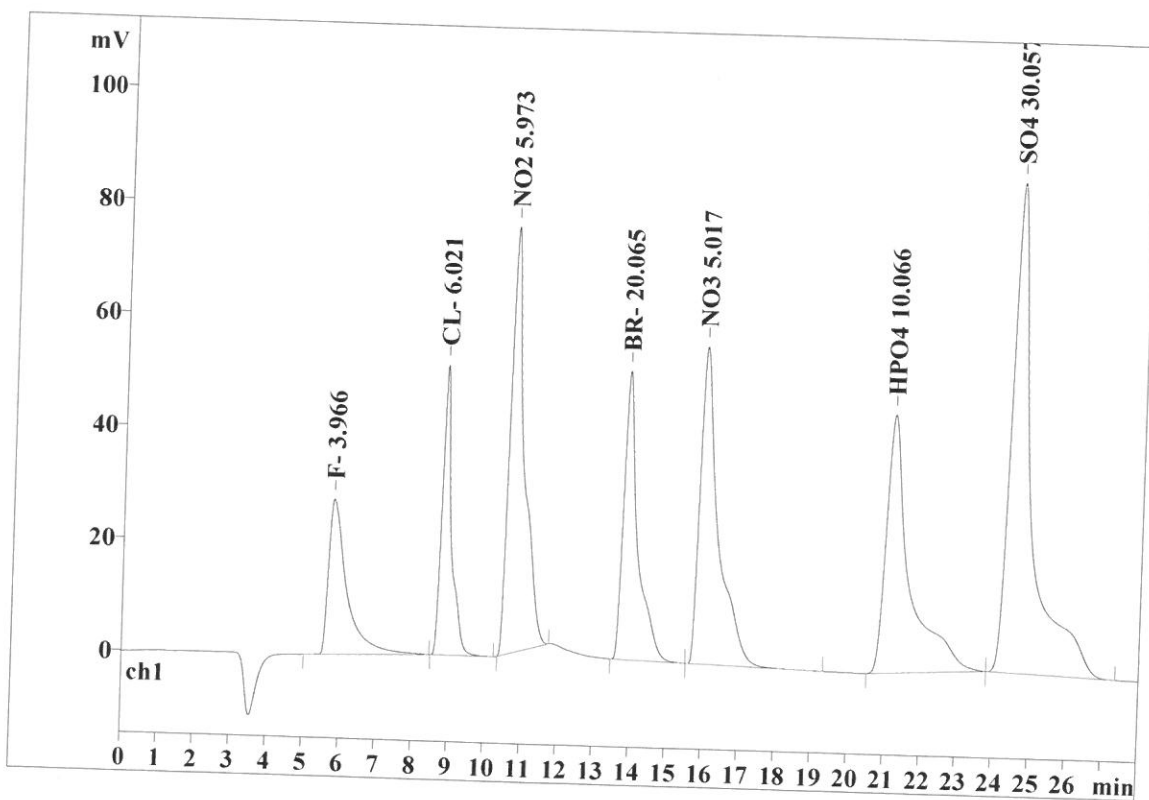

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.75	0.456	27.48	6.97	956.402	7.36
2	8.80	0.235	51.33	13.02	944.827	7.27
3	10.63	0.357	75.58	19.18	2068.005	15.92
4	13.82	0.345	51.07	12.96	1395.465	10.74
5	15.93	0.458	56.19	14.26	1996.590	15.37
6	21.14	0.511	45.69	11.59	2080.031	16.01
7	24.53	0.478	86.75	22.01	3551.905	27.34
7	28.00	0.406	394.09	100.00	12993.225	100.00

This report has been created by IC Net
METROHM LTD

Report date: 4/22/2020 9:13:13 AM
Printed by: wet


Ident: STD7
Analysis from: 4/21/2020 3:19:34 PM
File: _2020-04-21_

Last save: 4/21/2020 3:49:40 PM

Method: AnionsIC2-042120.mtw
Run operator: wet
Analysis number: 25081

Last save: 4/21/2020 2:26:

SAMPLE:
: AM/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

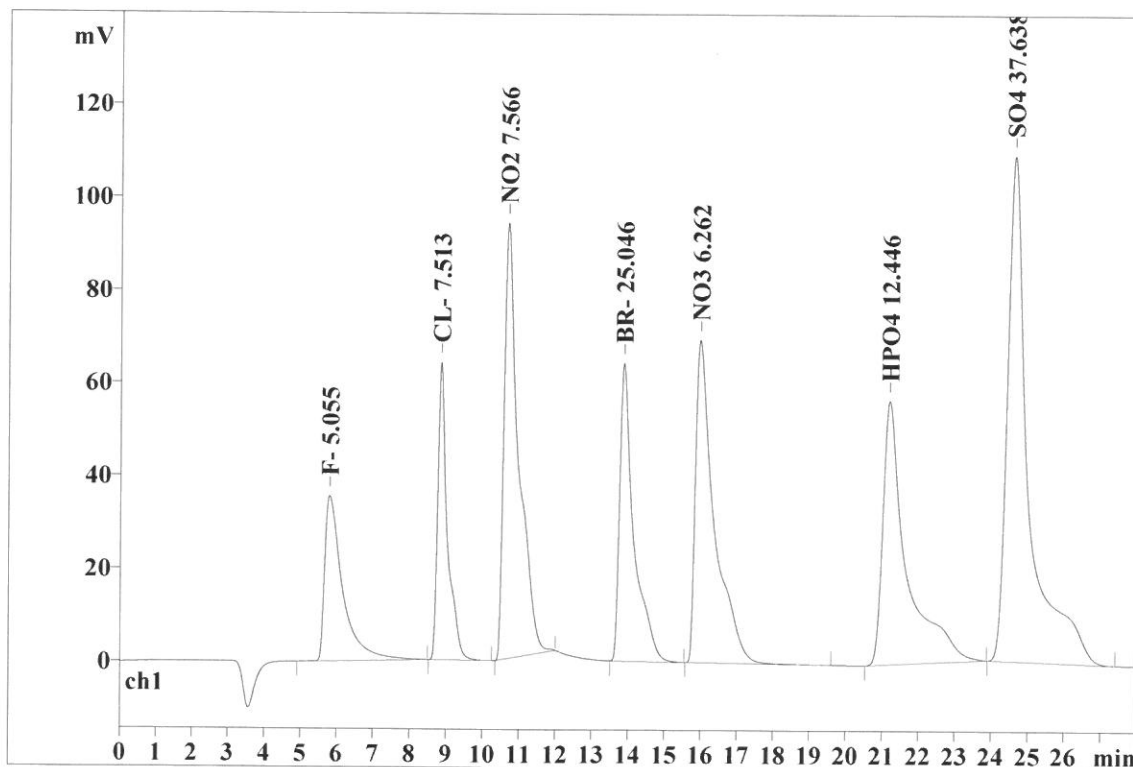

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.78	0.461	35.54	7.22	1226.058	7.51
2	8.82	0.236	64.04	13.01	1181.834	7.24
3	10.65	0.366	93.79	19.06	2634.122	16.13
4	13.85	0.344	64.08	13.02	1746.583	10.70
5	15.95	0.466	69.30	14.08	2498.760	15.30
6	21.18	0.512	56.70	11.52	2579.689	15.80
7	24.58	0.480	108.71	22.09	4459.685	27.32
7	28.00	0.409	492.16	100.00	16326.731	100.00

This report has been created by IC Net
METROHM LTD

Report date: 4/22/2020 9:13:21 AM
Printed by: wet


Ident: ICV
Analysis from: 4/21/2020 3:52:33 PM
File: _2020-04-21_

Last save: 4/21/2020 4:20:33 PM

Method: AnionsIC2-042120.mtw
Run operator: wet
Analysis number: 25082

Last save: 4/21/2020 3:48:

SAMPLE:
: AM/AP
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

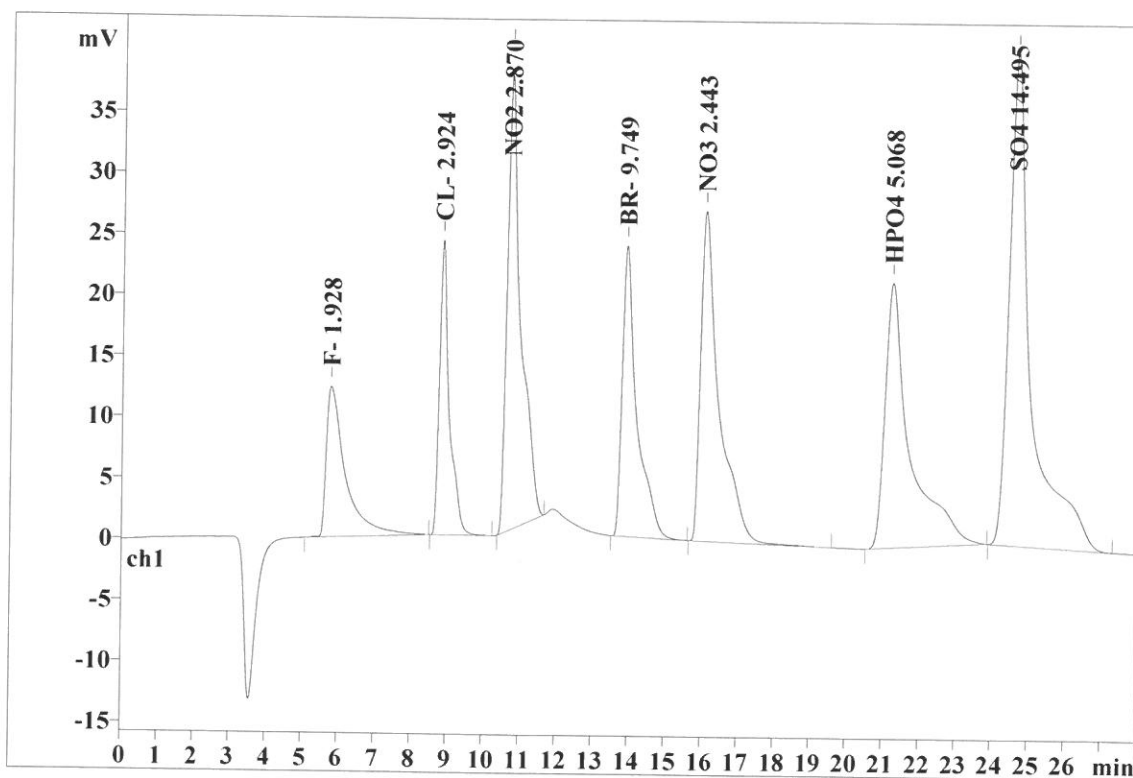

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.76	0.472	12.32	6.60	452.194	7.27
2	8.82	0.241	24.13	12.93	452.636	7.28
3	10.67	0.331	37.31	20.00	965.404	15.53
4	13.87	0.358	23.81	12.76	668.264	10.75
5	16.03	0.455	27.02	14.48	958.757	15.42
6	21.20	0.530	21.70	11.63	1030.594	16.58
7	24.58	0.486	40.29	21.60	1688.495	27.16
7	28.00	0.411	186.58	100.00	6216.343	100.00

This report has been created by IC Net
METROHM LTD

Report date: 4/22/2020 9:13:30 AM
Printed by: wet


Ident: ICB
Analysis from: 4/21/2020 4:23:33 PM
File: _2020-04-21_

Last save: 4/21/2020 4:58:13 PM

Method: AnionsIC2-042120.mtw
Run operator: wet
Analysis number: 25083

Last save: 4/21/2020 3:48:

SAMPLE:
:
Vial number: AM/AP
Volume: 10
Dilution: 20.0 µL
Amount: 1.00
1.0000

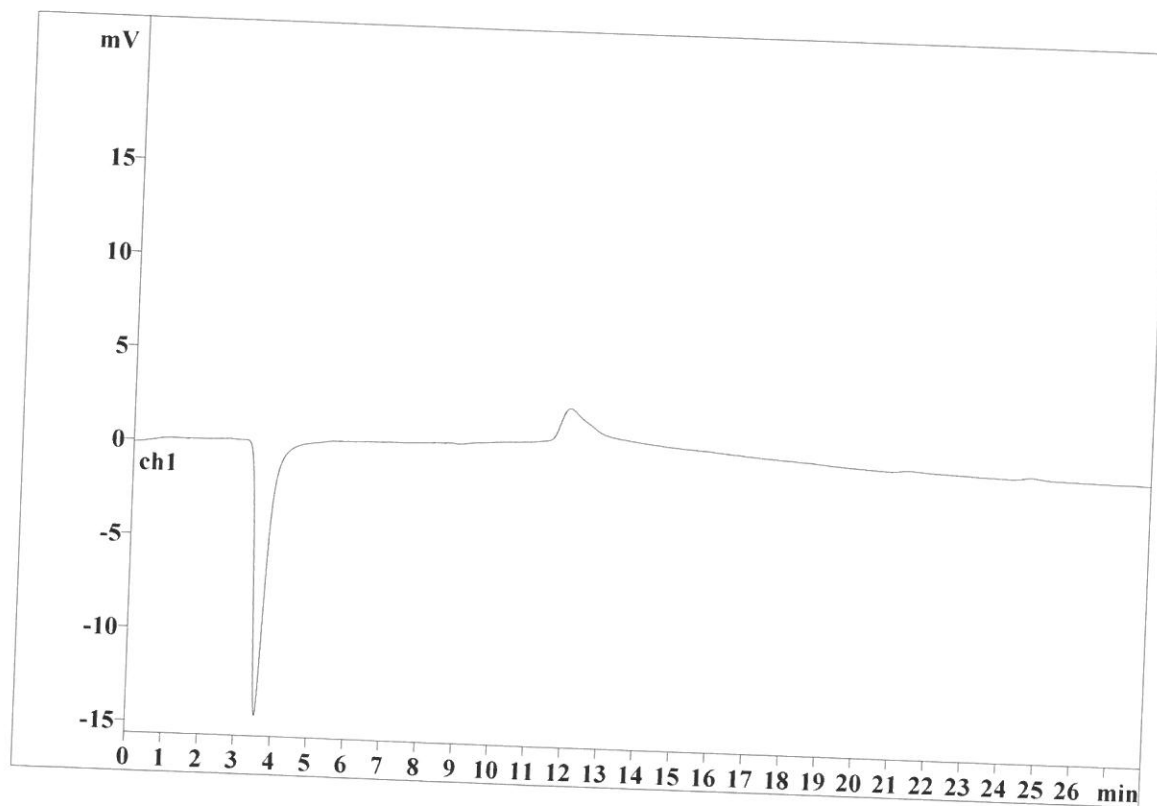

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 4/23/2020 10:51:18 AM
Printed by: wet


Ident: CCV
Analysis from: 4/22/2020 10:11:01 AM
File: _2020-04-22_

Last save: 4/23/2020 8:33:19 AM

Method: AnionsIC2-042120.mtw
Run operator: wet
Analysis number: 25091

Last save: 4/21/2020 4:58:

SAMPLE:
: AM/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.77	0.474	12.49	6.86	450.711	7.45
2	8.89	0.238	23.54	12.93	444.771	7.35
3	10.79	0.328	35.83	19.68	928.407	15.35
4	14.09	0.355	23.02	12.64	657.412	10.87
5	16.31	0.452	25.86	14.21	930.152	15.38
6	21.20	0.512	21.08	11.58	974.717	16.11
7	24.63	0.480	40.21	22.09	1662.944	27.49
7	28.00	0.406	182.03	100.00	6049.114	100.00

This report has been created by IC Net
METROHM LTD

Report date: 4/23/2020 10:51:35 AM
Printed by: wet


Ident: CCB
Analysis from: 4/22/2020 10:41:38 AM
File: _2020-04-22_

Last save: 4/22/2020 11:09:39 AM

Method: AnionsIC2-042120.mtw
Run operator: wet
Analysis number: 25092

Last save: 4/21/2020 4:58:

SAMPLE:
: AM/AP
Vial number: 3
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 4/23/2020 11:25:15 AM
Printed by: wet


Ident: LB108832BLW
Analysis from: 4/22/2020 11:12:17 AM
File: _2020-04-22_

Last save: 4/22/2020 4:48:53 PM

Method: AnionsIC2-042120.mtw
Run operator: wet
Analysis number: 25093

Last save: 4/21/2020 4:58:

SAMPLE:
: AM/AP
Vial number: 4
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 4/23/2020 11:25:31 AM
Printed by: wet


Ident: LB108832BSW
Analysis from: 4/22/2020 11:42:55 AM
File: _2020-04-22_

Last save: 4/23/2020 8:33:19 AM

Method: AnionsIC2-042120.mtw
Run operator: wet
Analysis number: 25094

Last save: 4/21/2020 4:58:

SAMPLE:
: AM/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.77	0.474	12.52	6.87	454.781	7.47
2	8.86	0.239	23.60	12.94	444.699	7.31
3	10.73	0.328	36.16	19.83	935.248	15.37
4	13.99	0.355	23.13	12.68	657.793	10.81
5	16.19	0.451	26.09	14.31	931.235	15.30
6	21.20	0.520	21.25	11.65	999.147	16.42
7	24.63	0.484	39.62	21.72	1662.830	27.32
7	28.00	0.407	182.38	100.00	6085.736	100.00

This report has been created by IC Net
METROHM LTD

Report date: 4/23/2020 11:25:40 AM
Printed by: wet


Ident: L2384-01
Analysis from: 4/22/2020 1:13:04 PM
File: _2020-04-22_

Last save: 4/22/2020 1:41:04 PM

Method: AnionsIC2-042120.mtw
Run operator: wet
Analysis number: 25096

Last save: 4/21/2020 4:58:

SAMPLE:
: AM/AP
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.91	0.223	0.99	99.82	18.089	100.00
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	0.00	0.000	0.00	0.00	0.000	0.00
7	28.00	0.032	0.99	99.82	18.089	100.00

This report has been created by IC Net
METROHM LTD

Report date: 4/23/2020 11:25:49 AM
Printed by: wet


Ident: L2384-01DUP
Analysis from: 4/22/2020 1:43:41 PM
File: _2020-04-22_

Last save: 4/23/2020 8:33:20 AM

Method: AnionsIC2-042120.mtw
Run operator: wet
Analysis number: 25097

Last save: 4/21/2020 4:58:

SAMPLE:
: AM/AP
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.90	0.224	0.95	100.00	17.235	100.00
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	0.00	0.000	0.00	0.00	0.000	0.00
7	28.00	0.032	0.95	100.00	17.235	100.00

This report has been created by IC Net
METROHM LTD

Report date: 4/23/2020 11:25:58 AM
Printed by: wet


Ident: L2384-01MS
Analysis from: 4/22/2020 2:14:19 PM
File: _2020-04-22_

Last save: 4/23/2020 8:33:20 AM

Method: AnionsIC2-042120.mtw
Run operator: wet
Analysis number: 25098

Last save: 4/21/2020 4:58:

SAMPLE:
: AM/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.74	0.499	11.93	6.43	458.838	7.47
2	8.81	0.228	25.68	13.84	474.783	7.73
3	10.67	0.314	36.33	19.58	935.639	15.23
4	13.92	0.344	23.61	12.73	667.290	10.86
5	16.10	0.441	26.80	14.45	958.330	15.60
6	21.10	0.510	20.27	10.93	950.076	15.46
7	24.52	0.477	40.88	22.04	1699.256	27.66
7	28.00	0.402	185.50	100.00	6144.211	100.00

This report has been created by IC Net
METROHM LTD

Report date: 4/23/2020 11:26:06 AM
Printed by: wet


Ident: L2384-01MSD
Analysis from: 4/22/2020 2:45:01 PM
File: _2020-04-22_

Last save: 4/22/2020 3:13:01 PM

Method: AnionsIC2-042120.mtw
Run operator: wet
Analysis number: 25099

Last save: 4/21/2020 4:58:

SAMPLE:
: AM/AP
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.75	0.491	11.30	6.35	429.708	7.30
2	8.83	0.228	24.51	13.78	454.688	7.72
3	10.70	0.317	34.71	19.52	898.625	15.26
4	13.93	0.342	22.76	12.80	641.006	10.88
5	16.11	0.436	25.82	14.52	914.268	15.52
6	21.18	0.510	19.68	11.07	921.369	15.64
7	24.61	0.479	39.04	21.96	1630.645	27.68
7	28.00	0.400	177.82	100.00	5890.310	100.00

This report has been created by IC Net
METROHM LTD

Report date: 4/23/2020 11:35:12 AM
Printed by: wet


Ident: L2182-07
Analysis from: 4/22/2020 3:15:38 PM
File: _2020-04-22_

Last save: 4/22/2020 4:07:57 PM

Method: AnionsIC2-042120.mtw
Run operator: wet
Analysis number: 25100

Last save: 4/21/2020 4:58:

SAMPLE:
: AM/AP
Vial number: 10
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.76	0.625	0.46	5.60	20.520	7.55
2	8.86	0.222	1.11	13.39	20.237	7.45
3	10.76	0.274	1.69	20.38	34.418	12.67
4	14.06	0.352	1.04	12.57	29.300	10.78
5	16.35	0.425	1.22	14.74	43.065	15.85
6	21.25	0.525	0.79	9.56	38.879	14.31
7	24.69	0.499	1.96	23.67	85.288	31.39
7	28.00	0.417	8.27	99.91	271.706	100.00

This report has been created by IC Net
METROHM LTD

Report date: 4/23/2020 11:36:44 AM
Printed by: wet


Ident: L2182-08
Analysis from: 4/22/2020 3:46:16 PM
File: _2020-04-22_

Last save: 4/22/2020 4:14:16 PM

Method: AnionsIC2-042120.mtw
Run operator: wet
Analysis number: 25101

Last save: 4/21/2020 4:58:

SAMPLE:
: AM/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.75	0.540	0.90	5.25	36.643	6.63
2	8.83	0.225	2.30	13.42	41.880	7.58
3	10.73	0.277	3.58	20.92	76.144	13.77
4	14.00	0.348	2.19	12.78	62.030	11.22
5	16.26	0.420	2.59	15.13	92.624	16.75
6	21.20	0.512	1.70	9.94	79.732	14.42
7	24.64	0.493	3.85	22.50	163.790	29.63
7	28.00	0.402	17.10	99.94	552.842	100.00

This report has been created by IC Net
METROHM LTD

Report date: 4/23/2020 11:37:22 AM
Printed by: wet


Ident: L2182-08RE
Analysis from: 4/22/2020 4:16:54 PM
File: _2020-04-22_

Last save: 4/23/2020 11:37:21 AM

Method: AnionsIC2-042120.mtw
Run operator: wet
Analysis number: 25102

Last save: 4/22/2020 4:08:

SAMPLE:
: AM/AP
Vial number: 12
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.74	0.519	1.85	5.29	72.921	6.47
2	8.83	0.225	4.67	13.34	85.687	7.60
3	10.71	0.286	7.27	20.76	162.755	14.44
4	13.96	0.343	4.50	12.85	126.216	11.20
5	16.20	0.413	5.25	15.01	177.979	15.79
6	21.21	0.514	3.75	10.72	174.956	15.52
7	24.64	0.489	7.71	22.02	326.827	28.99
7	28.00	0.399	35.00	99.99	1127.342	100.00

This report has been created by IC Net
METROHM LTD

Report date: 4/23/2020 11:37:30 AM
Printed by: wet


Ident: CCV
Analysis from: 4/22/2020 4:47:37 PM
File: _2020-04-22_

Last save: 4/23/2020 8:33:20 AM

Method: AnionsIC2-042120.mtw
Run operator: wet
Analysis number: 25103

Last save: 4/21/2020 4:58:

SAMPLE:
: AM/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.76	0.491	12.58	6.69	469.365	7.58
2	8.83	0.223	24.49	13.02	449.068	7.26
3	10.68	0.302	37.31	19.83	935.383	15.12
4	13.90	0.333	23.88	12.69	661.775	10.69
5	16.06	0.423	26.91	14.30	938.253	15.16
6	21.21	0.512	22.61	12.02	1061.766	17.16
7	24.66	0.480	40.34	21.44	1672.664	27.03
7	28.00	0.395	188.12	100.00	6188.273	100.00

This report has been created by IC Net
METROHM LTD

Report date: 4/23/2020 11:37:39 AM
Printed by: wet


Ident: CCB
Analysis from: 4/22/2020 5:18:15 PM
File: _2020-04-22_

Last save: 4/22/2020 5:46:15 PM

Method: AnionsIC2-042120.mtw
Run operator: wet
Analysis number: 25104

Last save: 4/22/2020 4:08:

SAMPLE:
: AM/AP
Vial number: 3
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000



Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD