

LB168946

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by :

Instrument ID : Konelab

4/30/2020 15:02

Deutsche
Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	93.941	0.0	0.071	
ICB1	0.488	0.0	0.003	
CCV1	234.816	0.0	0.172	
CCB1	0.493	0.0	0.003	
PB128587BL	0.328	0.0	0.003	
L2436-04	0.420	0.0	0.003	
L2436-04DUP	0.305	0.0	0.003	
L2452-02	0.230	0.0	0.003	
L2452-04	0.220	0.0	0.003	
L2452-06	0.138	0.0	0.003	
L2452-08	0.385	0.0	0.003	
CCV2	242.507	0.0	0.178	
CCB2	0.673	0.0	0.003	

N	13
Mean	44.226
SD	90.0682
CV%	203.65

Aquakem v. 7.2AQ1

Results from time period:

Thu Apr 30 14:55:08 2020

Thu Apr 30 15:01:55 2020

174

Sample Id	Sam/Ctr/c	Test short name	Test type	Result	Result unit	Result date and time
0.OPPBCN	A	REACTIVE CN	P	0.0106	µg/l	4/30/2020 12:21:49
5.OPPBCN	A	REACTIVE CN	P	5.0697	µg/l	4/30/2020 12:21:50
10PPBCN	A	REACTIVE CN	P	10.3002	µg/l	4/30/2020 12:21:51
50PPBCN	A	REACTIVE CN	P	49.2422	µg/l	4/30/2020 12:21:52
100PPBCN	A	REACTIVE CN	P	98.8416	µg/l	4/30/2020 12:21:53
250PPBCN	A	REACTIVE CN	P	252.4698	µg/l	4/30/2020 12:21:54
500PPBCN	A	REACTIVE CN	P	499.0658	µg/l	4/30/2020 12:21:55
ICV1	S	REACTIVE CN	P	93.941	µg/l	4/30/2020 14:55:09
ICB1	S	REACTIVE CN	P	0.4875	µg/l	4/30/2020 14:55:10
CCV1	S	REACTIVE CN	P	234.8161	µg/l	4/30/2020 14:55:13
CCB1	S	REACTIVE CN	P	0.493	µg/l	4/30/2020 14:55:14
PB128587BL	S	REACTIVE CN	P	0.328	µg/l	4/30/2020 14:55:17
L2436-04	S	REACTIVE CN	P	0.4202	µg/l	4/30/2020 14:55:18
L2436-04DUP	S	REACTIVE CN	P	0.3047	µg/l	4/30/2020 15:01:47
L2452-02	S	REACTIVE CN	P	0.2298	µg/l	4/30/2020 15:01:48
L2452-04	S	REACTIVE CN	P	0.2196	µg/l	4/30/2020 15:01:49
L2452-06	S	REACTIVE CN	P	0.1378	µg/l	4/30/2020 15:01:50
L2452-08	S	REACTIVE CN	P	0.3846	µg/l	4/30/2020 15:01:51
CCV2	S	REACTIVE CN	P	242.5075	µg/l	4/30/2020 15:01:53
CCB2	S	REACTIVE CN	P	0.6727	µg/l	4/30/2020 15:01:54

LB 108446

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : SK

Instrument ID : Konelab

4/30/2020 12:59


Test ^{Residue}
~~Total~~ CN

Accepted 4/30/2020 12:26

Factor 1387
Bias 0.003

Coeff. of det. 0.999956

Errors

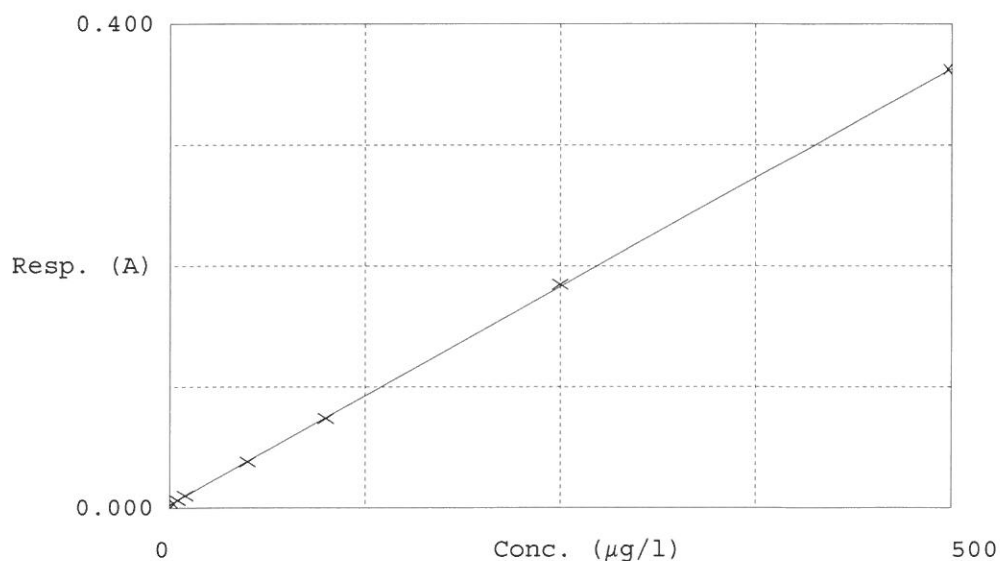

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	0.0106	0.0000	
2	5.0PPBCN	0.006	5.0697	5.0000	
3	10PPBCN	0.010	10.3002	10.0000	
4	50PPBCN	0.038	49.2422	50.0000	
5	100PPBCN	0.074	98.8416	100.0000	
6	250PPBCN	0.185	252.4698	250.0000	
7	500PPBCN	0.363	499.0658	500.0000	