

LB108971

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : JK

Instrument ID : Konelab

5/1/2020 12:12

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.032	0.0	0.111	
ICB1	-0.002	0.0	0.005	
CCV1	1.006	0.0	0.108	
CCB1	-0.001	0.0	0.005	
PB128552BL	-0.001	0.0	0.005	
PB128552BS	1.026	0.0	0.110	
L2182-10	0.024	0.0	0.007	
L2182-11	0.047	0.0	0.010	
L2430-01	0.040	0.0	0.009	
L2430-01DUP	0.041	0.0	0.009	
L2430-01MS	0.973	0.0	0.105	
L2430-01MSD	0.977	0.0	0.105	
CCV2	1.004	0.0	0.108	
CCB2	-0.002	0.0	0.005	

N	14
Mean	0.440
SD	0.5062
CV%	114.96

Aquakem v. 7.2AQ1

Results from time period:

Fri May 01 11:50:07 2020

Fri May 01 12:06:33 2020

DK

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0515	mg/l	5/1/2020 9:02:55	
0.1PPM	A	Phenolics-	P	0.109	mg/l	5/1/2020 9:02:56	
0.25PPM	A	Phenolics-	P	0.2477	mg/l	5/1/2020 9:02:57	
0.50PPM	A	Phenolics-	P	0.5006	mg/l	5/1/2020 9:02:58	
1.0PPM	A	Phenolics-	P	0.983	mg/l	5/1/2020 9:02:59	
2.0PPM	A	Phenolics-	P	2.0082	mg/l	5/1/2020 9:03:00	
ICV1	S	Phenolics-	P	1.0319	mg/l	5/1/2020 11:50:08	
ICB1	S	Phenolics-	P	-0.0015	mg/l	5/1/2020 11:50:09	
CCV1	S	Phenolics-	P	1.0064	mg/l	5/1/2020 11:50:12	
CCB1	S	Phenolics-	P	-0.0009	mg/l	5/1/2020 11:50:13	
PB128552BL	S	Phenolics-	P	-0.001	mg/l	5/1/2020 11:50:15	
PB128552BS	S	Phenolics-	P	1.0255	mg/l	5/1/2020 11:50:18	
L2182-10	S	Phenolics-	P	0.0239	mg/l	5/1/2020 12:00:11	
L2182-11	S	Phenolics-	P	0.0473	mg/l	5/1/2020 12:00:13	
L2430-01	S	Phenolics-	P	0.0403	mg/l	5/1/2020 12:00:17	
L2430-01DUP	S	Phenolics-	P	0.0407	mg/l	5/1/2020 12:00:18	
L2430-01MS	S	Phenolics-	P	0.9729	mg/l	5/1/2020 12:06:28	
L2430-01MSD	S	Phenolics-	P	0.9767	mg/l	5/1/2020 12:06:29	
CCV2	S	Phenolics-	P	1.0043	mg/l	5/1/2020 12:06:31	
CCB2	S	Phenolics-	P	-0.0025	mg/l	5/1/2020 12:06:32	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092

5/1/2020 10:10

Reviewed by : DL

Instrument ID : Konelab


Test Phenolics-

Accepted 5/1/2020 9:08

Factor 9.736
Bias 0.005

Coeff. of det. 0.999841

Errors

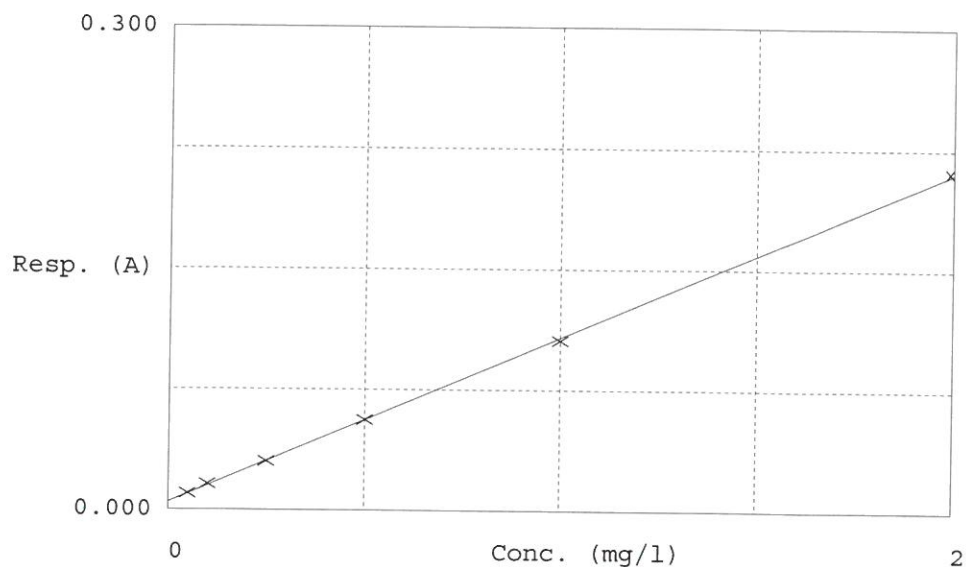

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.010	0.0515	0.0500	
2	Phenol-2	0.016	0.1090	0.1000	
3	Phenol-2	0.030	0.2477	0.2500	
4	Phenol-2	0.056	0.5006	0.5000	
5	Phenol-2	0.106	0.9830	1.0000	
6	Phenol-2	0.211	2.0082	2.0000	