

L67109 011

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : Dk

Instrument ID : Konelab

5/5/2020 15:01

Test: ^{Positive}
~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.078	0.0	0.065	
ICB1	1.118	0.0	0.003	
CCV1	261.198	0.0	0.175	
CCB1	1.197	0.0	0.003	
PB128650BL	0.978	0.0	0.003	
L2122-15	0.867	0.0	0.003	
L2122-15DUP	0.854	0.0	0.003	
L2463-06	0.905	0.0	0.003	
L2463-12	0.809	0.0	0.003	
L2463-15	0.827	0.0	0.003	
L2463-19	0.777	0.0	0.003	
L2463-22	0.796	0.0	0.003	
L2466-01	0.876	0.0	0.003	
CCV2	245.288	0.0	0.164	
CCB2	0.552	0.0	0.003	

N	15
Mean	40.741
SD	89.5835
CV%	219.88

Aquakem v. 7.2AQ1

Results from time period:

Tue May 05 14:35:20 2020

Tue May 05 14:45:43 2020

1)h

Sample Id	Sam/Ctr/c	Test short name	Test type	Result	Result unit	Result date and time
0.OPPBCN	A	REACTIVE CN	P	-0.5482	µg/l	5/5/2020 12:11:35
5.OPPBCN	A	REACTIVE CN	P	5.3614	µg/l	5/5/2020 12:11:36
10PPBCN	A	REACTIVE CN	P	10.9023	µg/l	5/5/2020 12:11:37
50PPBCN	A	REACTIVE CN	P	48.2446	µg/l	5/5/2020 12:11:38
100PPBCN	A	REACTIVE CN	P	96.1777	µg/l	5/5/2020 12:11:39
250PPBCN	A	REACTIVE CN	P	257.8878	µg/l	5/5/2020 12:11:40
500PPBCN	A	REACTIVE CN	P	496.9744	µg/l	5/5/2020 12:11:41
ICV1	S	REACTIVE CN	P	94.0776	µg/l	5/5/2020 14:35:20
ICB1	S	REACTIVE CN	P	1.1184	µg/l	5/5/2020 14:35:22
CCV1	S	REACTIVE CN	P	261.1981	µg/l	5/5/2020 14:35:24
CCB1	S	REACTIVE CN	P	1.1975	µg/l	5/5/2020 14:35:27
PB128650BL	S	REACTIVE CN	P	0.9775	µg/l	5/5/2020 14:35:29
L2122-15	S	REACTIVE CN	P	0.867	µg/l	5/5/2020 14:35:30
L2122-15DUP	S	REACTIVE CN	P	0.8542	µg/l	5/5/2020 14:42:56
L2463-06	S	REACTIVE CN	P	0.905	µg/l	5/5/2020 14:42:57
L2463-12	S	REACTIVE CN	P	0.8086	µg/l	5/5/2020 14:42:58
L2463-15	S	REACTIVE CN	P	0.8265	µg/l	5/5/2020 14:42:59
L2463-19	S	REACTIVE CN	P	0.7773	µg/l	5/5/2020 14:43:00
L2463-22	S	REACTIVE CN	P	0.7956	µg/l	5/5/2020 14:43:01
L2466-01	S	REACTIVE CN	P	0.876	µg/l	5/5/2020 14:43:02
CCV2	S	REACTIVE CN	P	245.2877	µg/l	5/5/2020 14:43:04
CCB2	S	REACTIVE CN	P	0.5522	µg/l	5/5/2020 14:45:43

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092

Reviewed by : DL

Instrument ID : Konelab

5/5/2020 15:02


Test ^{Revise} Total CN

Accepted 5/5/2020 12:12

Factor 1518
Bias 0.003

Coeff. of det. 0.999561

Errors

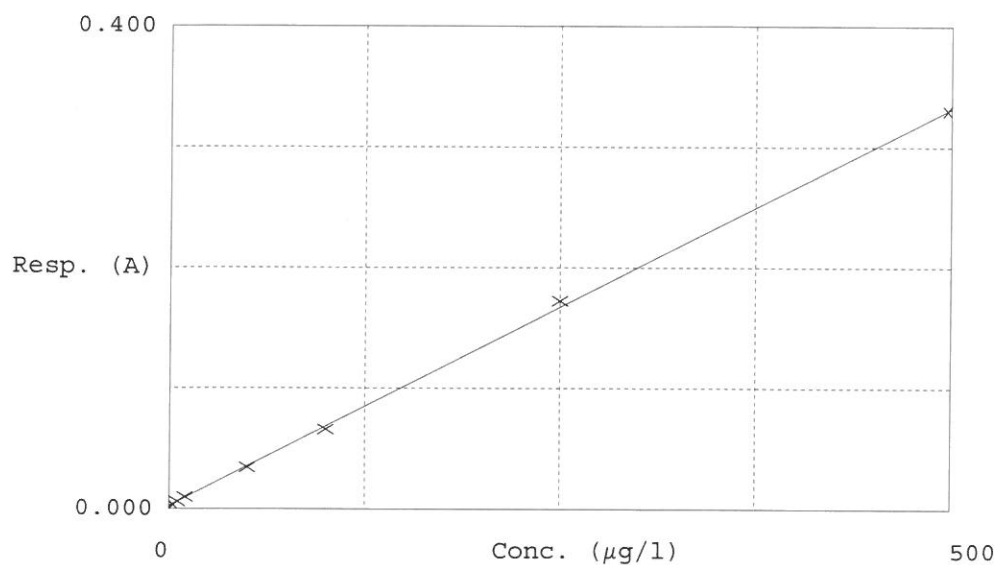

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	-0.5482	0.0000	
2	5.0PPBCN	0.006	5.3614	5.0000	
3	10PPBCN	0.010	10.9023	10.0000	
4	50PPBCN	0.034	48.2446	50.0000	
5	100PPBCN	0.066	96.1777	100.0000	
6	250PPBCN	0.173	257.8878	250.0000	
7	500PPBCN	0.330	496.9744	500.0000	