

LB109067

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : Dh

Instrument ID : Konelab

5/8/2020 9:47

Test: Ammonia-N

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.002	0.0	0.224	
ICB1	0.004	0.0	0.040	
CCV1	0.985	0.0	0.221	
CCB1	-0.001	0.0	0.039	
L2472-05DLX5	1.501	0.0	0.316	
CCV2	0.991	0.0	0.222	
CCB2	0.011	0.0	0.041	

N	7
Mean	0.642
SD	0.6227
CV%	97.00

Aquakem v. 7.2AQ1

Results from time period:

Fri May 08 09:00:02 2020

Fri May 08 09:38:00 2020

De

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.1PPM	A	Ammonia-I	P	0.0961	mg/l	5/8/2020 9:00:02	
0.2PPM	A	Ammonia-I	P	0.1984	mg/l	5/8/2020 9:00:03	
0.4PPM	A	Ammonia-I	P	0.4089	mg/l	5/8/2020 9:00:04	
1.0PPM	A	Ammonia-I	P	1.0222	mg/l	5/8/2020 9:00:05	
1.3PPM	A	Ammonia-I	P	1.2942	mg/l	5/8/2020 9:00:06	
2.0PPM	A	Ammonia-I	P	2.0136	mg/l	5/8/2020 9:00:07	
ICV1	S	Ammonia-I	P	1.0022	mg/l	5/8/2020 9:33:05	
ICB1	S	Ammonia-I	P	0.0041	mg/l	5/8/2020 9:33:06	
CCV1	S	Ammonia-I	P	0.9847	mg/l	5/8/2020 9:33:09	
CCB1	S	Ammonia-I	P	-0.001	mg/l	5/8/2020 9:33:10	
L2472-05DLX5	S	Ammonia-I	P	1.5012	mg/l	5/8/2020 9:33:12	
CCV2	S	Ammonia-I	P	0.9913	mg/l	5/8/2020 9:33:15	
CCB2	S	Ammonia-I	P	0.0108	mg/l	5/8/2020 9:37:59	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : Dk

Instrument ID : Konelab

5/8/2020 9:00


Test Ammonia-N

Accepted 5/8/2020 9:00

Factor 5.421
Bias 0.039

Coeff. of det. 0.999167

Errors

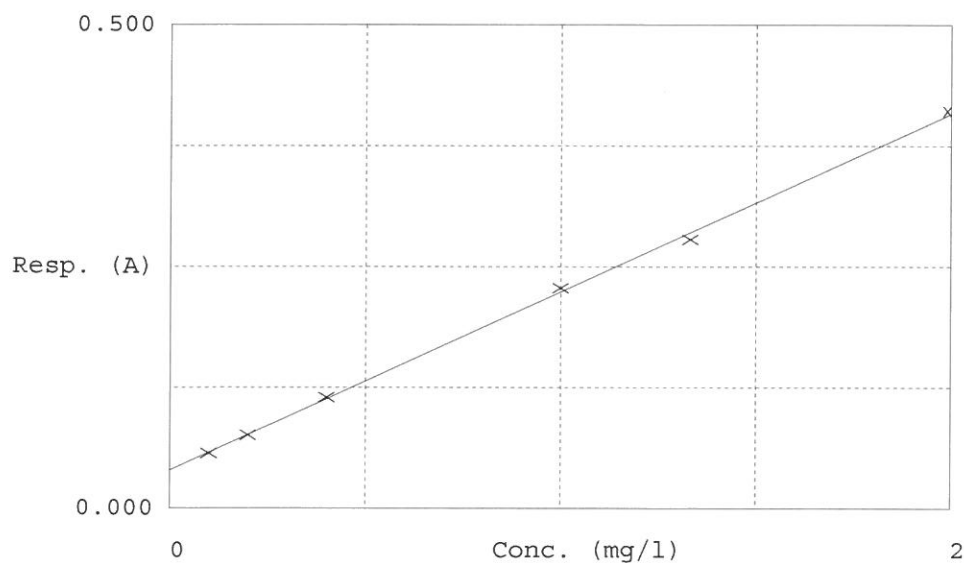

	Calibrator	Response	Calc. con.	Conc.	Errors
1	NH3-2PPM	0.057	0.0961	0.1000	
2	NH3-2PPM	0.076	0.1984	0.2000	
3	NH3-2PPM	0.115	0.4089	0.4000	
4	NH3-2PPM	0.228	1.0222	1.0000	
5	NH3-2PPM	0.278	1.2942	1.3333	
6	NH3-2PPM	0.411	2.0136	2.0000	