

LB109071

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : Dh

Instrument ID : Konelab

5/8/2020 12:42

Test: Total CN

Mg/L

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	102.680	0.0	0.071	
ICB1	-0.529	0.0	0.003	
CCV1	238.491	0.0	0.161	
CCB1	-0.737	0.0	0.003	
PB128714BL	-0.719	0.0	0.003	
PB128714BS	94.998	0.0	0.066	
MIDPB128714	241.645	0.0	0.163	
L2116-01MS	49.354	0.0	0.036	
L2116-01MSD	49.301	0.0	0.036	
L2116-01	0.083	0.0	0.004	
L2116-01DUP	0.162	0.0	0.004	
L2182-12	1.826	0.0	0.005	
CCV2	274.770	0.0	0.185	
CCB2	-0.549	0.0	0.003	

N	14
Mean	75.056
SD	102.4101
CV%	136.45

Aquakem v. 7.2AQ1

Results from time period:

Fri May 08 11:50:43 2020

Fri May 08 12:35:29 2020

36

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	-1.1665	µg/l	5/8/2020 11:50:43	
5.OPPBCN	A	Total CN	P	4.6114	µg/l	5/8/2020 11:50:44	
10PPBCN	A	Total CN	P	11.1029	µg/l	5/8/2020 11:50:45	
50PPBCN	A	Total CN	P	51.7022	µg/l	5/8/2020 11:50:46	
100PPBCN	A	Total CN	P	100.9623	µg/l	5/8/2020 11:50:47	
250PPBCN	A	Total CN	P	246.337	µg/l	5/8/2020 11:50:48	
500PPBCN	A	Total CN	P	501.4507	µg/l	5/8/2020 11:50:49	
ICV1	S	Total CN	P	102.6804	µg/l	5/8/2020 12:23:06	
ICB1	S	Total CN	P	-0.5286	µg/l	5/8/2020 12:23:09	
CCV1	S	Total CN	P	238.4911	µg/l	5/8/2020 12:23:11	
CCB1	S	Total CN	P	-0.7366	µg/l	5/8/2020 12:23:12	
PB128714BL	S	Total CN	P	-0.7192	µg/l	5/8/2020 12:23:15	
PB128714BS	S	Total CN	P	94.998	µg/l	5/8/2020 12:23:16	
MIDPB128714	S	Total CN	P	241.6452	µg/l	5/8/2020 12:30:39	
L2116-01MS	S	Total CN	P	49.3539	µg/l	5/8/2020 12:30:41	
L2116-01MSD	S	Total CN	P	49.3005	µg/l	5/8/2020 12:30:42	
L2116-01	S	Total CN	P	0.0826	µg/l	5/8/2020 12:30:44	
L2116-01DUP	S	Total CN	P	0.1622	µg/l	5/8/2020 12:30:45	
L2182-12	S	Total CN	P	1.8263	µg/l	5/8/2020 12:35:25	
CCV2	S	Total CN	P	274.7702	µg/l	5/8/2020 12:35:26	
CCB2	S	Total CN	P	-0.549	µg/l	5/8/2020 12:35:29	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092

Reviewed by : DK

Instrument ID : Konelab

5/8/2020 11:51


Test Total CN

Accepted 5/8/2020 11:51

Factor 1511
Bias 0.003

Coeff. of det. 0.999893

Errors

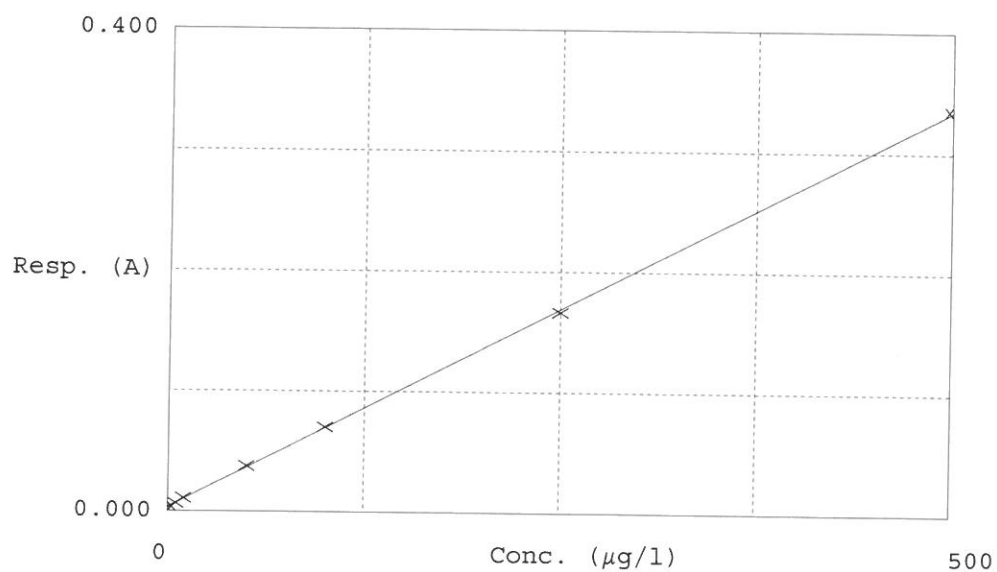

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-1.1665	0.0000	
2	5.0PPBCN	0.007	4.6114	5.0000	
3	10PPBCN	0.011	11.1029	10.0000	
4	50PPBCN	0.038	51.7022	50.0000	
5	100PPBCN	0.070	100.9623	100.0000	
6	250PPBCN	0.166	246.3370	250.0000	
7	500PPBCN	0.335	501.4507	500.0000	