

LB109272

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : DK

Instrument ID : Konelab

5/22/2020 10:23

Test: Phenolics- mg/L

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.046	0.0	0.108	
ICB1	-0.013	0.0	0.003	
CCV1	1.022	0.0	0.106	
CCB1	-0.008	0.0	0.004	
PB129050BL	-0.011	0.0	0.004	
PB129050BS	1.059	0.0	0.109	
L2734-01	-0.008	0.0	0.004	
L2734-02	-0.007	0.0	0.004	
L2734-03	-0.007	0.0	0.004	
L2734-03DUP	-0.009	0.0	0.004	
L2734-03MS	1.010	0.0	0.104	
L2734-03MSD	1.000	0.0	0.103	
L2734-04	-0.008	0.0	0.004	
L2734-05	-0.010	0.0	0.004	
CCV2	1.009	0.0	0.104	
CCB2	-0.009	0.0	0.004	

N	16
Mean	0.379
SD	0.5167
CV%	136.51

Aquakem v. 7.2AQ1

Results from time period:

Fri May 22 09:36:10 2020

Fri May 22 10:20:41 2020

De

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0512	mg/l	5/22/2020 9:36:10	
0.1PPM	A	Phenolics-	P	0.1067	mg/l	5/22/2020 9:36:11	
0.25PPM	A	Phenolics-	P	0.2458	mg/l	5/22/2020 9:36:12	
0.50PPM	A	Phenolics-	P	0.4939	mg/l	5/22/2020 9:36:13	
1.0PPM	A	Phenolics-	P	1.0015	mg/l	5/22/2020 9:36:14	
2.0PPM	A	Phenolics-	P	2.0009	mg/l	5/22/2020 9:36:15	
ICV1	S	Phenolics-	P	1.0456	mg/l	5/22/2020 10:05:42	
ICB1	S	Phenolics-	P	-0.0128	mg/l	5/22/2020 10:05:45	
CCV1	S	Phenolics-	P	1.0221	mg/l	5/22/2020 10:05:47	
CCB1	S	Phenolics-	P	-0.0082	mg/l	5/22/2020 10:05:48	
PB129050BL	S	Phenolics-	P	-0.0107	mg/l	5/22/2020 10:05:51	
PB129050BS	S	Phenolics-	P	1.0588	mg/l	5/22/2020 10:05:52	
L2734-01	S	Phenolics-	P	-0.008	mg/l	5/22/2020 10:15:44	
L2734-02	S	Phenolics-	P	-0.0071	mg/l	5/22/2020 10:15:45	
L2734-03	S	Phenolics-	P	-0.0066	mg/l	5/22/2020 10:15:46	
L2734-03DUP	S	Phenolics-	P	-0.0086	mg/l	5/22/2020 10:15:47	
L2734-03MS	S	Phenolics-	P	1.0096	mg/l	5/22/2020 10:15:49	
L2734-03MSD	S	Phenolics-	P	1.0002	mg/l	5/22/2020 10:15:50	
L2734-04	S	Phenolics-	P	-0.0083	mg/l	5/22/2020 10:15:53	
L2734-05	S	Phenolics-	P	-0.0096	mg/l	5/22/2020 10:15:54	
CCV2	S	Phenolics-	P	1.0087	mg/l	5/22/2020 10:20:38	
CCB2	S	Phenolics-	P	-0.009	mg/l	5/22/2020 10:20:39	

LB109278

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : De

Instrument ID : Konelab

5/22/2020 9:37


Test Phenolics-

Accepted 5/22/2020 9:37

Factor 10.13
Bias 0.005

Coeff. of det. 0.999963

Errors

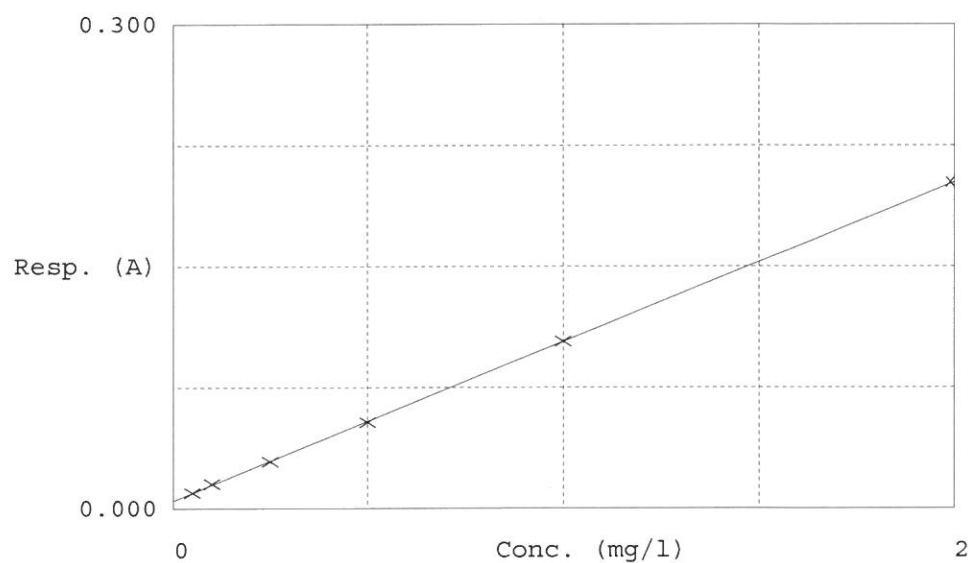

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.010	0.0512	0.0500	
2	Phenol-2	0.015	0.1067	0.1000	
3	Phenol-2	0.029	0.2458	0.2500	
4	Phenol-2	0.053	0.4939	0.5000	
5	Phenol-2	0.104	1.0015	1.0000	
6	Phenol-2	0.202	2.0009	2.0000	