

LB109560

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : *dh*

Instrument ID : Konelab

6/11/2020 12:40

Test: Total CN

Mg/l

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.511	0.0	0.075	
ICB1	1.338	0.0	0.003	
CCV1	237.482	0.0	0.181	
CCB1	1.273	0.0	0.003	
PB129488BL	1.315	0.0	0.003	
PB129488BS	96.302	0.0	0.075	
LOWPB129488	11.385	0.0	0.011	
HIGHPB129488	490.469	0.0	0.372	
L2810-01	2.272	0.0	0.004	
L2810-01DUP	1.213	0.0	0.003	
L2810-01MS	43.403	0.0	0.035	
L2810-01MSD	41.834	0.0	0.034	
L2817-01	2.264	0.0	0.004	
L2819-01	1.825	0.0	0.004	
CCV2	236.716	0.0	0.181	
CCB2	1.388	0.0	0.004	
L2954-02	3.535	0.0	0.005	
L2970-02	1.474	0.0	0.004	
L2972-01	1.954	0.0	0.004	
L2972-04	1.800	0.0	0.004	
L2972-07	2.037	0.0	0.004	
CCV3	247.560	0.0	0.189	
CCB3	1.448	0.0	0.004	

N	23
Mean	66.382
SD	123.4592
CV%	185.98

Aquakem v. 7.2AQ1

Results from time period:

Thu Jun 11 12:19:48 2020

Thu Jun 11 12:39:17 2020

dh

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	0.7596	µg/l	6/11/2020 10:40:06	
5.OPPBCN	A	Total CN	P	5.9755	µg/l	6/11/2020 10:40:07	
10PPBCN	A	Total CN	P	10.8239	µg/l	6/11/2020 10:40:08	
50PPBCN	A	Total CN	P	49.8348	µg/l	6/11/2020 10:40:09	
100PPBCN	A	Total CN	P	99.9571	µg/l	6/11/2020 10:40:10	
250PPBCN	A	Total CN	P	245.3004	µg/l	6/11/2020 10:40:11	
500PPBCN	A	Total CN	P	502.3487	µg/l	6/11/2020 10:40:12	
ICV1	S	Total CN	P	96.5109	µg/l	6/11/2020 12:19:49	
ICB1	S	Total CN	P	1.3376	µg/l	6/11/2020 12:19:50	
CCV1	S	Total CN	P	237.4822	µg/l	6/11/2020 12:19:53	
CCB1	S	Total CN	P	1.2732	µg/l	6/11/2020 12:19:55	
PB129488BL	S	Total CN	P	1.3152	µg/l	6/11/2020 12:19:56	
PB129488BS	S	Total CN	P	96.3022	µg/l	6/11/2020 12:19:58	
LOWPB129488	S	Total CN	P	11.3854	µg/l	6/11/2020 12:27:23	
HIGHPB129488	S	Total CN	P	490.4693	µg/l	6/11/2020 12:27:25	
L2810-01	S	Total CN	P	2.2716	µg/l	6/11/2020 12:27:27	
L2810-01DUP	S	Total CN	P	1.2129	µg/l	6/11/2020 12:27:28	
L2810-01MS	S	Total CN	P	43.4026	µg/l	6/11/2020 12:27:29	
L2810-01MSD	S	Total CN	P	41.8337	µg/l	6/11/2020 12:27:31	
L2817-01	S	Total CN	P	2.2636	µg/l	6/11/2020 12:34:55	
L2819-01	S	Total CN	P	1.8253	µg/l	6/11/2020 12:34:56	
CCV2	S	Total CN	P	236.7158	µg/l	6/11/2020 12:34:57	
CCB2	S	Total CN	P	1.3876	µg/l	6/11/2020 12:35:00	
L2954-02	S	Total CN	P	3.5347	µg/l	6/11/2020 12:35:01	
L2970-02	S	Total CN	P	1.4742	µg/l	6/11/2020 12:35:02	
L2972-01	S	Total CN	P	1.9543	µg/l	6/11/2020 12:35:03	
L2972-04	S	Total CN	P	1.8001	µg/l	6/11/2020 12:35:04	
L2972-07	S	Total CN	P	2.0366	µg/l	6/11/2020 12:35:05	
CCV3	S	Total CN	P	247.5598	µg/l	6/11/2020 12:39:15	
CCB3	S	Total CN	P	1.4475	µg/l	6/11/2020 12:39:17	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by :

Instrument ID : Konelab

6/11/2020 11:05


Test Total CN

Accepted 6/11/2020 10:40

Factor 1329
Bias 0.002

Coeff. of det. 0.999855

Errors

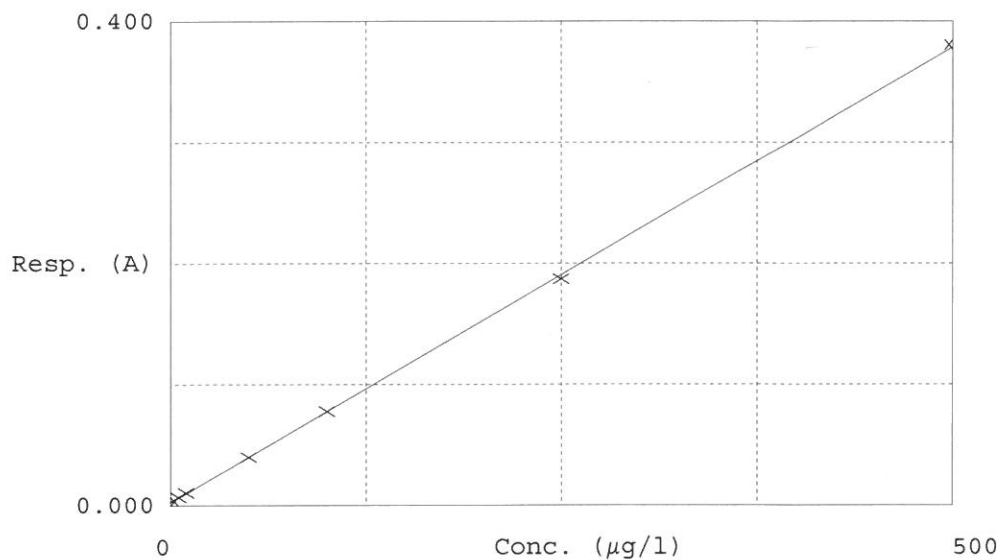

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	0.7596	0.0000	
2	5.0PPBCN	0.007	5.9755	5.0000	
3	10PPBCN	0.011	10.8239	10.0000	
4	50PPBCN	0.040	49.8348	50.0000	
5	100PPBCN	0.078	99.9571	100.0000	
6	250PPBCN	0.187	245.3004	250.0000	
7	500PPBCN	0.381	502.3487	500.0000	