

LB109750

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : *ix*

Instrument ID : Konelab

6/26/2020 11:52

Test: Total CN

Mg / L

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.033	0.0	0.071	
ICB1	1.204	0.0	0.002	
CCV1	241.163	0.0	0.182	
CCB1	1.135	0.0	0.002	
PB129805BL	1.105	0.0	0.001	
PB129805BS	94.345	0.0	0.072	
MIDPB129805	241.417	0.0	0.182	
L3125-01	1.265	0.0	0.002	
L3125-01DUP	1.295	0.0	0.002	
L3125-01MS	8.520	0.0	0.007	
L3125-01MSD	8.357	0.0	0.007	
CCV2	246.119	0.0	0.186	
CCB2	1.182	0.0	0.002	

N	13
Mean	72.395
SD	102.7847
CV%	141.98

Aquakem v. 7.2AQ1

Results from time period:

Fri Jun 26 10:11:15 2020

Fri Jun 26 11:50:13 2020

15

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	0.7006	µg/l	6/26/2020 11:06:19	
5.0PPBCN	A	Total CN	P	5.7347	µg/l	6/26/2020 11:06:20	
10PPBCN	A	Total CN	P	10.8302	µg/l	6/26/2020 11:06:21	
50PPBCN	A	Total CN	P	49.7182	µg/l	6/26/2020 11:06:22	
100PPBCN	A	Total CN	P	97.0969	µg/l	6/26/2020 11:06:23	
250PPBCN	A	Total CN	P	250.6691	µg/l	6/26/2020 11:06:24	
500PPBCN	A	Total CN	P	500.2503	µg/l	6/26/2020 11:06:25	
ICV1	S	Total CN	P	94.0335	µg/l	6/26/2020 11:42:58	
ICB1	S	Total CN	P	1.204	µg/l	6/26/2020 11:43:00	
CCV1	S	Total CN	P	241.1628	µg/l	6/26/2020 11:43:01	
CCB1	S	Total CN	P	1.1349	µg/l	6/26/2020 11:43:03	
PB129805BL	S	Total CN	P	1.1048	µg/l	6/26/2020 11:43:05	
PB129805BS	S	Total CN	P	94.3446	µg/l	6/26/2020 11:43:06	
MIDPB129805	S	Total CN	P	241.4173	µg/l	6/26/2020 11:43:07	
L3125-01	S	Total CN	P	1.2652	µg/l	6/26/2020 11:50:04	
L3125-01DUP	S	Total CN	P	1.2949	µg/l	6/26/2020 11:50:05	
L3125-01MS	S	Total CN	P	8.5198	µg/l	6/26/2020 11:50:08	
L3125-01MSD	S	Total CN	P	8.3572	µg/l	6/26/2020 11:50:09	
CCV2	S	Total CN	P	246.1187	µg/l	6/26/2020 11:50:11	
CCB2	S	Total CN	P	1.182	µg/l	6/26/2020 11:50:13	

LB109750

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : ijk

Instrument ID : Konelab

6/26/2020 11:06


Test Total CN

Accepted 6/26/2020 11:06

Factor 1331
Bias 0.001

Coeff. of det. 0.999948

Errors

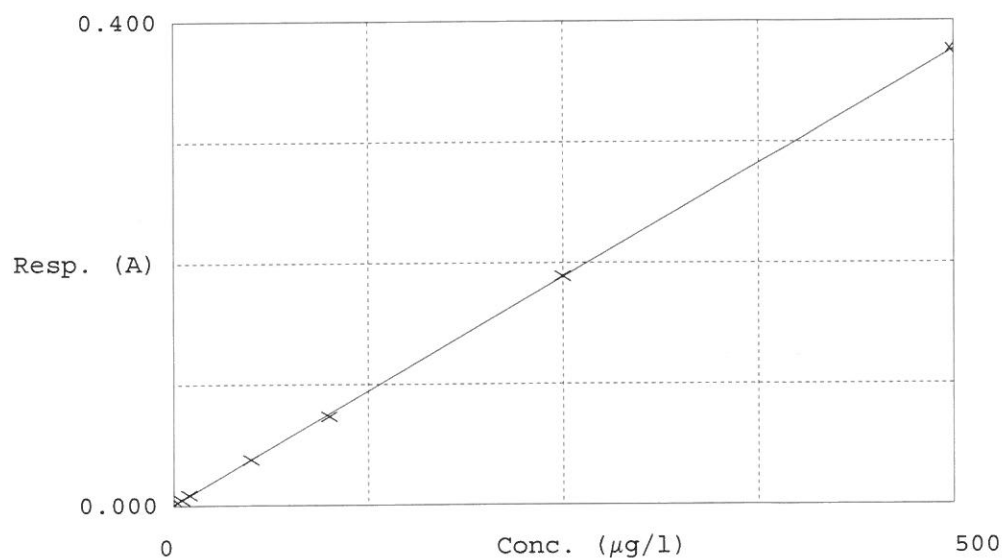

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	0.7006	0.0000	
2	5.0PPBCN	0.005	5.7347	5.0000	
3	10PPBCN	0.009	10.8302	10.0000	
4	50PPBCN	0.038	49.7182	50.0000	
5	100PPBCN	0.074	97.0969	100.0000	
6	250PPBCN	0.189	250.6691	250.0000	
7	500PPBCN	0.377	500.2503	500.0000	