

LB109775

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : Dk

Instrument ID : Konelab

6/29/2020 10:19

Test: Phenolics- mg/L

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.023	0.0	0.110	
ICB1	0.002	0.0	0.005	
CCV1	1.024	0.0	0.110	
CCB1	0.004	0.0	0.005	
PB129808BL	0.001	0.0	0.004	
PB129808BS	1.021	0.0	0.110	
L3125-01	0.002	0.0	0.004	
L3125-01DUP	0.004	0.0	0.005	
L3125-01MS	0.901	0.0	0.098	
L3125-01MSD	0.904	0.0	0.098	
CCV2	1.011	0.0	0.109	
CCB2	0.002	0.0	0.004	

N	12
Mean	0.492
SD	0.5126
CV%	104.23

Aquakem v. 7.2AQ1

Results from time period:

Mon Jun 29 09:36:50 2020

Mon Jun 29 10:17:29 2020

Dh

Sample Id	Sam/Ctr/c	Test short na	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0529	mg/l	6/29/2020 9:36:50	
0.1PPM	A	Phenolics-	P	0.108	mg/l	6/29/2020 9:36:51	
0.25PPM	A	Phenolics-	P	0.2493	mg/l	6/29/2020 9:36:52	
0.50PPM	A	Phenolics-	P	0.5095	mg/l	6/29/2020 9:36:53	
1.0PPM	A	Phenolics-	P	0.9661	mg/l	6/29/2020 9:36:54	
2.0PPM	A	Phenolics-	P	2.0142	mg/l	6/29/2020 9:36:55	
ICV1	S	Phenolics-	P	1.0233	mg/l	6/29/2020 10:09:39	
ICB1	S	Phenolics-	P	0.0024	mg/l	6/29/2020 10:09:40	
CCV1	S	Phenolics-	P	1.0245	mg/l	6/29/2020 10:09:42	
CCB1	S	Phenolics-	P	0.0045	mg/l	6/29/2020 10:09:45	
PB129808BL	S	Phenolics-	P	0.0013	mg/l	6/29/2020 10:09:47	
PB129808BS	S	Phenolics-	P	1.0213	mg/l	6/29/2020 10:09:48	
L3125-01	S	Phenolics-	P	0.0021	mg/l	6/29/2020 10:17:20	
L3125-01DUP	S	Phenolics-	P	0.0037	mg/l	6/29/2020 10:17:21	
L3125-01MS	S	Phenolics-	P	0.9013	mg/l	6/29/2020 10:17:22	
L3125-01MSD	S	Phenolics-	P	0.9041	mg/l	6/29/2020 10:17:23	
CCV2	S	Phenolics-	P	1.0114	mg/l	6/29/2020 10:17:27	
CCB2	S	Phenolics-	P	0.0016	mg/l	6/29/2020 10:17:29	

LB109775

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : Dh

Instrument ID : Konelab

6/29/2020 9:37


Test Phenolics-

Accepted 6/29/2020 9:37

Factor 9.651
Bias 0.004

Coeff. of det. 0.999459

Errors

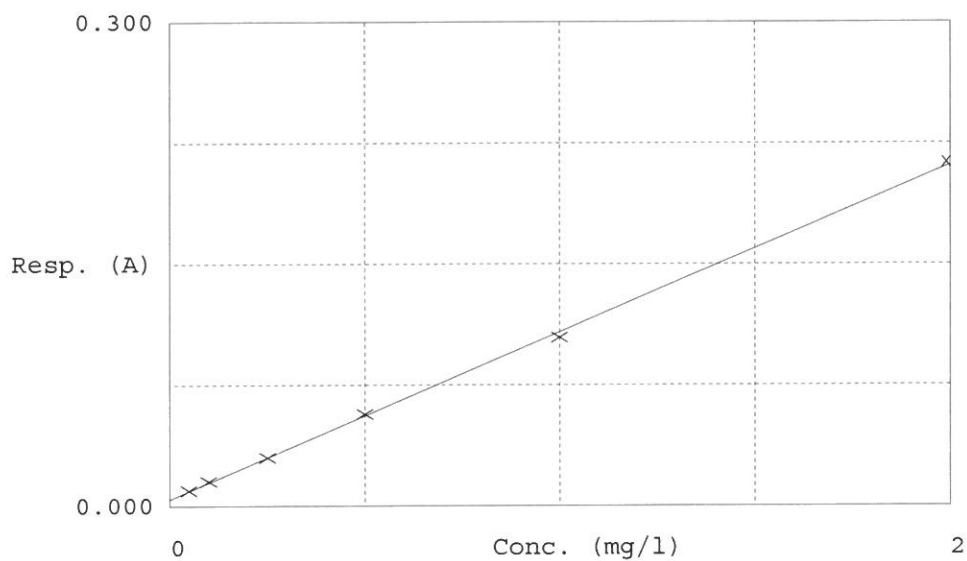

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.010	0.0529	0.0500	
2	Phenol-2	0.015	0.1080	0.1000	
3	Phenol-2	0.030	0.2493	0.2500	
4	Phenol-2	0.057	0.5095	0.5000	
5	Phenol-2	0.104	0.9661	1.0000	
6	Phenol-2	0.213	2.0142	2.0000	