

LB109815

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : DL

Instrument ID : Konelab

7/8/2020 16:54

Test: Phenolics- mg/L

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.004	0.0	0.112	
ICB1	0.002	0.0	0.004	
CCV1	1.011	0.0	0.113	
CCB1	0.005	0.0	0.005	
PB129919BL	0.001	0.0	0.004	
PB129919BS	1.009	0.0	0.113	
L3194-01	0.002	0.0	0.004	
L3194-01DUP	0.001	0.0	0.004	
L3194-01MS	0.939	0.0	0.105	
L3194-01MSD	0.939	0.0	0.105	
L3216-10	0.026	0.0	0.007	
L3216-11	0.046	0.0	0.009	
CCV2	1.000	0.0	0.112	
CCB2	0.002	0.0	0.004	

N	14
Mean	0.428
SD	0.5005
CV%	117.04

Aquakem v. 7.2AQ1

Results from time period:

Wed Jul 08 15:51:32 2020

Wed Jul 08 17:13:19 2020

De

Sample Id	Sam/Ctr/c	Test short name	Test type	Result	Result unit	Result date and time
0.05PPM	A	Phenolics-	P	0.0497	mg/l	7/8/2020 15:51:32
0.1PPM	A	Phenolics-	P	0.1015	mg/l	7/8/2020 15:51:33
0.25PPM	A	Phenolics-	P	0.2494	mg/l	7/8/2020 15:51:34
0.50PPM	A	Phenolics-	P	0.4992	mg/l	7/8/2020 15:51:35
1.0PPM	A	Phenolics-	P	0.9999	mg/l	7/8/2020 15:51:36
2.0PPM	A	Phenolics-	P	2.0002	mg/l	7/8/2020 15:51:37
ICV1	S	Phenolics-	P	1.0042	mg/l	7/8/2020 16:36:49
ICB1	S	Phenolics-	P	0.002	mg/l	7/8/2020 16:36:50
CCV1	S	Phenolics-	P	1.0113	mg/l	7/8/2020 16:36:51
CCB1	S	Phenolics-	P	0.0047	mg/l	7/8/2020 16:36:52
PB129919BL	S	Phenolics-	P	0.0013	mg/l	7/8/2020 16:36:53
PB129919BS	S	Phenolics-	P	1.0094	mg/l	7/8/2020 16:36:54
L3194-01	S	Phenolics-	P	0.0016	mg/l	7/8/2020 16:36:55
L3194-01DUP	S	Phenolics-	P	0.0013	mg/l	7/8/2020 16:36:56
L3194-01MS	S	Phenolics-	P	0.939	mg/l	7/8/2020 16:36:57
L3194-01MSD	S	Phenolics-	P	0.9393	mg/l	7/8/2020 16:36:58
L3216-10	S	Phenolics-	P	0.0255	mg/l	7/8/2020 16:37:00
L3216-11	S	Phenolics-	P	0.0457	mg/l	7/8/2020 16:46:53
CCV2	S	Phenolics-	P	1	mg/l	7/8/2020 16:46:57
CCB2	S	Phenolics-	P	0.0018	mg/l	7/8/2020 16:46:58

LB109915

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : Dh

Instrument ID : Konelab

7/8/2020 16:45


Test Phenolics-

Accepted 7/8/2020 15:52

Factor 9.28
Bias 0.004

Coeff. of det. 0.999999

Errors

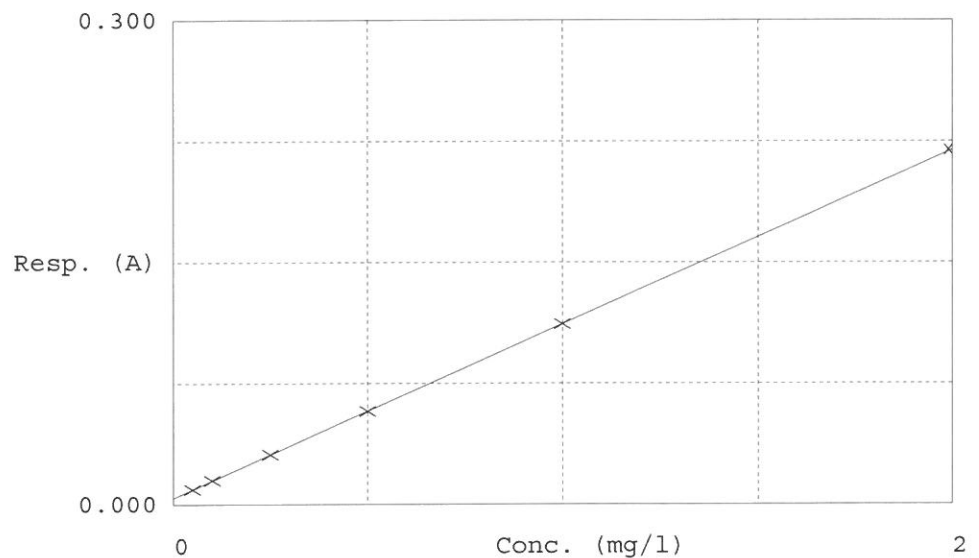

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.009	0.0497	0.0500	
2	Phenol-2	0.015	0.1015	0.1000	
3	Phenol-2	0.031	0.2494	0.2500	
4	Phenol-2	0.058	0.4992	0.5000	
5	Phenol-2	0.112	0.9999	1.0000	
6	Phenol-2	0.220	2.0002	2.0000	