

LB110031

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : DA

Instrument ID : Konelab

7/15/2020 11:25

Test: ^{perme} Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	98.493	0.0	0.082	
ICB1	-0.397	0.0	0.002	
CCV1	242.939	0.0	0.198	
CCB1	-0.211	0.0	0.002	
PB130266BL	-0.389	0.0	0.002	
L3183-10	-0.513	0.0	0.002	
L3183-10DUP	-0.363	0.0	0.002	
L3187-08	-0.544	0.0	0.002	
L3188-10	-0.492	0.0	0.002	
L3288-01	-0.515	0.0	0.002	
L3300-04	-0.349	0.0	0.002	
L3300-08	-0.554	0.0	0.002	
CCV2	258.491	0.0	0.211	
CCB2	-0.248	0.0	0.002	

N	14
Mean	42.525
SD	92.0797
CV%	216.53

Aquakem v. 7.2AQ1

Results from time period:

Wed Jul 15 10:44:24 2020

Du

Wed Jul 15 11:23:11 2020

Sample Id	Sam/Ctr/c/	Test short name	Test type	Result	Result unit	Result date and time
0.OPPBCN	A	REACTIVE CN	P	-0.7556	µg/l	7/15/2020 10:44:24
5.OPPBCN	A	REACTIVE CN	P	4.228	µg/l	7/15/2020 10:44:25
10PPBCN	A	REACTIVE CN	P	9.527	µg/l	7/15/2020 10:44:26
50PPBCN	A	REACTIVE CN	P	48.7329	µg/l	7/15/2020 10:44:27
100PPBCN	A	REACTIVE CN	P	102.6223	µg/l	7/15/2020 10:44:28
250PPBCN	A	REACTIVE CN	P	252.0517	µg/l	7/15/2020 10:44:29
500PPBCN	A	REACTIVE CN	P	498.5936	µg/l	7/15/2020 10:44:30
ICV1	S	REACTIVE CN	P	98.4927	µg/l	7/15/2020 11:19:18
ICB1	S	REACTIVE CN	P	-0.3969	µg/l	7/15/2020 11:19:19
CCV1	S	REACTIVE CN	P	242.9392	µg/l	7/15/2020 11:19:20
CCB1	S	REACTIVE CN	P	-0.2109	µg/l	7/15/2020 11:19:21
PB130266BL	S	REACTIVE CN	P	-0.3893	µg/l	7/15/2020 11:19:22
L3183-10	S	REACTIVE CN	P	-0.5134	µg/l	7/15/2020 11:19:23
L3183-10DUP	S	REACTIVE CN	P	-0.3634	µg/l	7/15/2020 11:19:24
L3187-08	S	REACTIVE CN	P	-0.544	µg/l	7/15/2020 11:19:25
L3188-10	S	REACTIVE CN	P	-0.4919	µg/l	7/15/2020 11:19:26
L3288-01	S	REACTIVE CN	P	-0.515	µg/l	7/15/2020 11:19:27
L3300-04	S	REACTIVE CN	P	-0.3492	µg/l	7/15/2020 11:19:28
L3300-08	S	REACTIVE CN	P	-0.5543	µg/l	7/15/2020 11:23:09
CCV2	S	REACTIVE CN	P	258.4905	µg/l	7/15/2020 11:23:10
CCB2	S	REACTIVE CN	P	-0.2483	µg/l	7/15/2020 11:23:11

LB110031

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : De

Instrument ID : Konelab

7/15/2020 10:54


Test Total CN

Accepted 7/15/2020 10:54

Factor 1241
 Bias 0.003

Coeff. of det. 0.999922

Errors

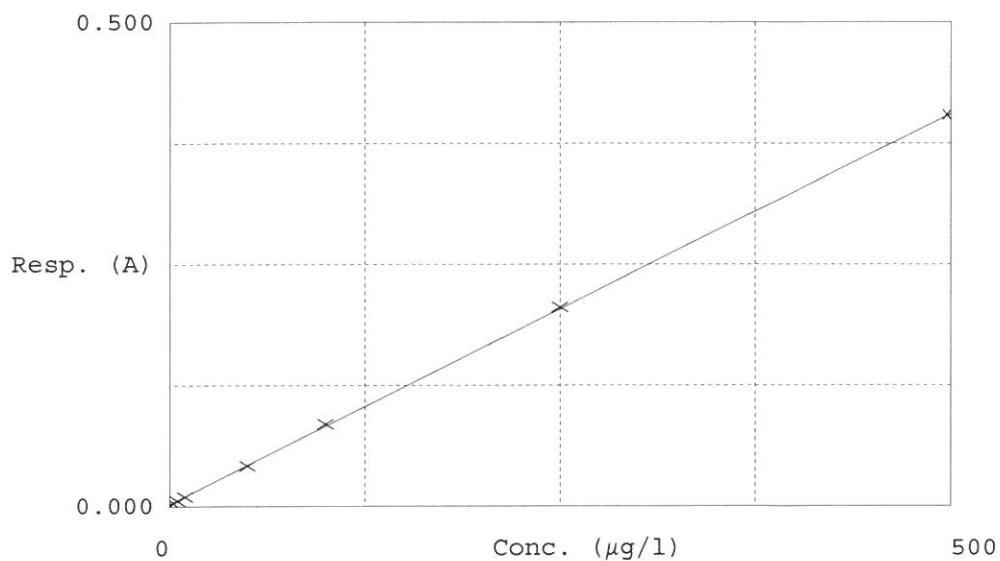

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	-0.7556	0.0000	
2	5.0PPBCN	0.006	4.2280	5.0000	
3	10PPBCN	0.010	9.5270	10.0000	
4	50PPBCN	0.042	48.7329	50.0000	
5	100PPBCN	0.085	102.6223	100.0000	
6	250PPBCN	0.206	252.0517	250.0000	
7	500PPBCN	0.404	498.5936	500.0000	