

LB 110056

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : D

Instrument ID : Konelab

7/16/2020 14:31

Test: ^{Peach}~~Total~~ CN *Myk*

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.228	0.0	0.083	
ICB1	-0.085	0.0	0.002	
CCV1	241.030	0.0	0.203	
CCB1	0.017	0.0	0.002	
PB130255BL	-0.048	0.0	0.002	
L3183-17	-0.020	0.0	0.002	
L3183-17DUP	0.016	0.0	0.002	
L3184-12	-0.127	0.0	0.002	
L3315-04	-0.052	0.0	0.002	
L3315-08	0.071	0.0	0.002	
CCV2	240.288	0.0	0.202	
CCB2	-0.301	0.0	0.002	

N	12
Mean	48.168
SD	94.1204
CV%	195.40

Aquakem v. 7.2AQ1

Results from time period:

Thu Jul 16 14:26:53 2020

Thu Jul 16 14:29:41 2020

176

Sample Id	Sam/Ctr/c/	Test short name	Test type	Result	Result unit	Result date and time
0.OPPBCN	A	REACTIVE CN	P	-0.6038	µg/l	7/16/2020 13:07:05
5.OPPBCN	A	REACTIVE CN	P	4.5093	µg/l	7/16/2020 13:07:06
10PPBCN	A	REACTIVE CN	P	9.4599	µg/l	7/16/2020 13:07:07
50PPBCN	A	REACTIVE CN	P	48.1446	µg/l	7/16/2020 13:07:08
100PPBCN	A	REACTIVE CN	P	101.7728	µg/l	7/16/2020 13:07:09
250PPBCN	A	REACTIVE CN	P	253.7409	µg/l	7/16/2020 13:07:10
500PPBCN	A	REACTIVE CN	P	497.9762	µg/l	7/16/2020 13:07:11
ICV1	S	REACTIVE CN	P	97.2277	µg/l	7/16/2020 14:26:53
ICB1	S	REACTIVE CN	P	-0.0847	µg/l	7/16/2020 14:26:54
CCV1	S	REACTIVE CN	P	241.0298	µg/l	7/16/2020 14:26:55
CCB1	S	REACTIVE CN	P	0.0174	µg/l	7/16/2020 14:26:56
PB130255BL	S	REACTIVE CN	P	-0.048	µg/l	7/16/2020 14:26:57
L3183-17	S	REACTIVE CN	P	-0.0204	µg/l	7/16/2020 14:26:58
L3183-17DUP	S	REACTIVE CN	P	0.0161	µg/l	7/16/2020 14:26:59
L3184-12	S	REACTIVE CN	P	-0.1266	µg/l	7/16/2020 14:27:00
L3315-04	S	REACTIVE CN	P	-0.0524	µg/l	7/16/2020 14:27:01
L3315-08	S	REACTIVE CN	P	0.0713	µg/l	7/16/2020 14:27:02
CCV2	S	REACTIVE CN	P	240.2882	µg/l	7/16/2020 14:27:03
CCB2	S	REACTIVE CN	P	-0.3011	µg/l	7/16/2020 14:29:41

LB110056

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : Sh

Instrument ID : Konelab

7/16/2020 15:14


Test Total CN

Accepted 7/16/2020 13:07

Factor 1201
Bias 0.002

Coeff. of det. 0.999876

Errors

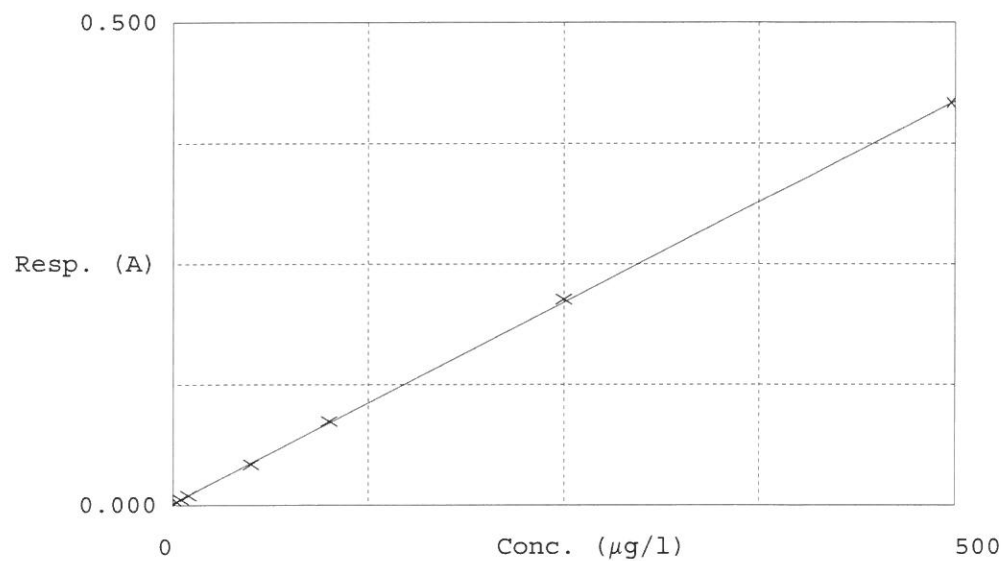

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	-0.6038	0.0000	
2	5.0PPBCN	0.006	4.5093	5.0000	
3	10PPBCN	0.010	9.4599	10.0000	
4	50PPBCN	0.042	48.1446	50.0000	
5	100PPBCN	0.087	101.7728	100.0000	
6	250PPBCN	0.214	253.7409	250.0000	
7	500PPBCN	0.417	497.9762	500.0000	