

=====

LB11081
=====

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : dy

Instrument ID : Konelab

7/17/2020 12:46
-----Test: Total CN *My LC*

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	98.985	0.0	0.080	
ICB1	-0.635	0.0	0.001	
CCV1	246.961	0.0	0.197	
CCB1	-0.365	0.0	0.001	
PB130281BL	-0.594	0.0	0.001	
PB130281BS	99.467	0.0	0.080	
LOWPB130281	9.437	0.0	0.009	
HIGHPB130281	488.031	0.0	0.388	
L3334-01X10	49.577	0.0	0.041	
L3334-01DUPX10	49.085	0.0	0.041	
L3334-01MSX10	62.709	0.0	0.051	
L3334-01MSDX10	64.093	0.0	0.052	
L3334-05X10	53.398	0.0	0.044	
L3334-06	3.006	0.0	0.004	
CCV2	262.371	0.0	0.210	
CCB2	-0.878	0.0	0.001	

N	16
Mean	92.790
SD	133.1144
CV%	143.46

Aquakem v. 7.2AQ1

Results from time period:

Fri Jul 17 11:40:53 2020

Fri Jul 17 12:46:02 2020

7h

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time
0.OPPBCN	A	Total CN	P	-0.8909	µg/l	7/17/2020 11:40:53
5.OPPBCN	A	Total CN	P	4.1543	µg/l	7/17/2020 11:40:54
10PPBCN	A	Total CN	P	11.309	µg/l	7/17/2020 11:40:55
50PPBCN	A	Total CN	P	47.4186	µg/l	7/17/2020 11:40:56
100PPBCN	A	Total CN	P	100.317	µg/l	7/17/2020 11:40:57
250PPBCN	A	Total CN	P	255.0299	µg/l	7/17/2020 11:40:58
500PPBCN	A	Total CN	P	497.6621	µg/l	7/17/2020 11:40:59
ICV1	S	Total CN	P	98.9851	µg/l	7/17/2020 12:21:44
ICB1	S	Total CN	P	-0.6354	µg/l	7/17/2020 12:21:45
CCV1	S	Total CN	P	246.9607	µg/l	7/17/2020 12:21:46
CCB1	S	Total CN	P	-0.3654	µg/l	7/17/2020 12:21:47
PB130281BL	S	Total CN	P	-0.5939	µg/l	7/17/2020 12:21:48
PB130281BS	S	Total CN	P	99.4673	µg/l	7/17/2020 12:21:49
LOWPB130281	S	Total CN	P	9.4373	µg/l	7/17/2020 12:21:50
HIGHPB130281	S	Total CN	P	488.0307	µg/l	7/17/2020 12:21:51
L3334-01X10	S	Total CN	P	49.5766	µg/l	7/17/2020 12:21:52
L3334-01DUPX10	S	Total CN	P	49.0845	µg/l	7/17/2020 12:21:53
L3334-01MSX10	S	Total CN	P	62.7091	µg/l	7/17/2020 12:21:54
L3334-01MSDX10	S	Total CN	P	64.0929	µg/l	7/17/2020 12:26:31
L3334-05X10	S	Total CN	P	53.3981	µg/l	7/17/2020 12:26:32
L3334-06	S	Total CN	P	3.0062	µg/l	7/17/2020 12:46:00
CCV2	S	Total CN	P	262.3715	µg/l	7/17/2020 12:46:01
CCB2	S	Total CN	P	-0.8779	µg/l	7/17/2020 12:46:02

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : Dk

Instrument ID : Konelab

7/17/2020 13:09


Test Total CN

Accepted 7/17/2020 11:46

Factor 1262
Bias 0.002

Coeff. of det. 0.999802

Errors

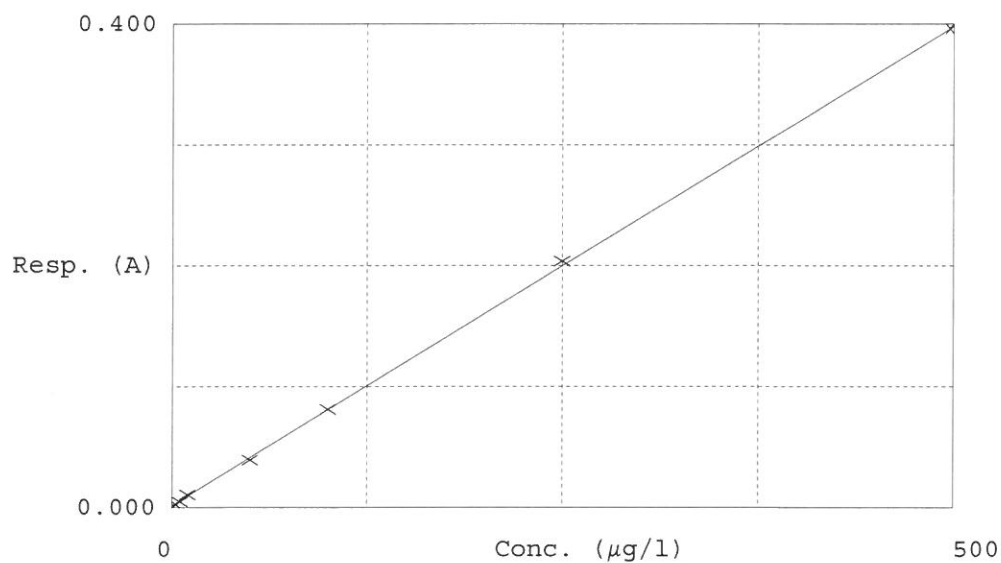

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	-0.8909	0.0000	
2	5.0PPBCN	0.005	4.1543	5.0000	
3	10PPBCN	0.011	11.3090	10.0000	
4	50PPBCN	0.039	47.4186	50.0000	
5	100PPBCN	0.081	100.3170	100.0000	
6	250PPBCN	0.204	255.0299	250.0000	
7	500PPBCN	0.396	497.6621	500.0000	