

LB11072

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092

Reviewed by : dh

Instrument ID : Konelab

7/23/2020 15:34

Test: Phenolics-

mg/L

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.025	0.0	0.116	
ICB1	0.002	0.0	0.006	
CCV1	1.011	0.0	0.115	
CCB1	-0.006	0.0	0.005	
PB130193BL	-0.000	0.0	0.006	
PB130193BS	1.020	0.0	0.116	
L3358-01	0.003	0.0	0.006	
L3358-01DUP	0.001	0.0	0.006	
L3358-01MS	0.918	0.0	0.105	
L3358-01MSD	0.914	0.0	0.104	
L3216-12	0.035	0.0	0.010	
CCV2	1.008	0.0	0.114	
CCB2	-0.002	0.0	0.006	

N	13
Mean	0.456
SD	0.5087
CV%	111.56

Aquakem v. 7.2AQ1

Results from time period:

Thu Jul 23 14:26:44 2020

Thu Jul 23 15:33:39 2020

D^a

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0546	mg/l	7/23/2020 14:26:44	
0.1PPM	A	Phenolics-	P	0.1038	mg/l	7/23/2020 14:26:45	
0.25PPM	A	Phenolics-	P	0.2456	mg/l	7/23/2020 14:26:46	
0.50PPM	A	Phenolics-	P	0.4971	mg/l	7/23/2020 14:26:47	
1.0PPM	A	Phenolics-	P	0.9959	mg/l	7/23/2020 14:26:48	
2.0PPM	A	Phenolics-	P	2.003	mg/l	7/23/2020 14:26:49	
ICV1	S	Phenolics-	P	1.025	mg/l	7/23/2020 14:53:49	
ICB1	S	Phenolics-	P	0.0023	mg/l	7/23/2020 14:53:50	
CCV1	S	Phenolics-	P	1.0107	mg/l	7/23/2020 14:53:51	
CCB1	S	Phenolics-	P	-0.0062	mg/l	7/23/2020 14:53:52	
PB130193BL	S	Phenolics-	P	-0.0001	mg/l	7/23/2020 14:53:53	
PB130193BS	S	Phenolics-	P	1.0201	mg/l	7/23/2020 14:53:54	
L3358-01	S	Phenolics-	P	0.0027	mg/l	7/23/2020 14:53:59	
L3358-01DUP	S	Phenolics-	P	0.0006	mg/l	7/23/2020 14:54:00	
L3358-01MS	S	Phenolics-	P	0.918	mg/l	7/23/2020 15:00:07	
L3358-01MSD	S	Phenolics-	P	0.9141	mg/l	7/23/2020 15:00:08	
L3216-12	S	Phenolics-	P	0.0347	mg/l	7/23/2020 15:33:36	
CCV2	S	Phenolics-	P	1.0082	mg/l	7/23/2020 15:33:38	
CCB2	S	Phenolics-	P	-0.0021	mg/l	7/23/2020 15:33:39	

LB110172

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : D^h

Instrument ID : Konelab

7/23/2020 14:29


Test Phenolics-

Accepted 7/23/2020 14:29

Factor 9.293
Bias 0.006

Coeff. of det. 0.999968

Errors

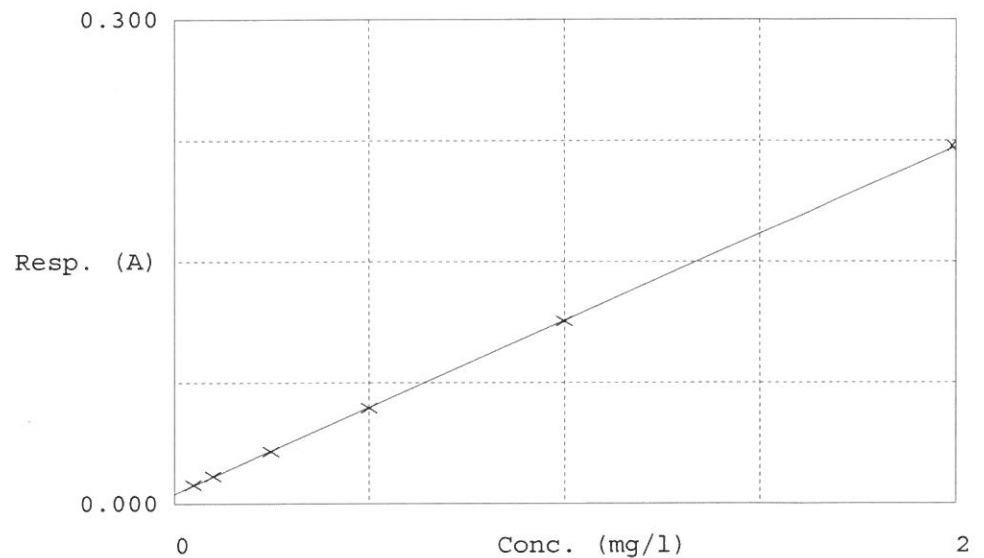

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.012	0.0546	0.0500	
2	Phenol-2	0.017	0.1038	0.1000	
3	Phenol-2	0.032	0.2456	0.2500	
4	Phenol-2	0.059	0.4971	0.5000	
5	Phenol-2	0.113	0.9959	1.0000	
6	Phenol-2	0.222	2.0030	2.0000	