

LB110328

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AM

Instrument ID : Konelab

7/31/2020 17:37

Test: CNEPA-NEW

Sample Id	Result	Dil. 1 +	Response	Errors
ICV ICV	95.497	0.0	0.104	
ICB ICB	1.238	0.0	0.008	
CCV001 CCV001	243.058	0.0	0.256	
CCB001 CCB001	1.380	0.0	0.008	
PB130566BL PBW56	1.070	0.0	0.007	
L3421-02	1.713	0.0	0.008	
L3421-03	2.463	0.0	0.009	
L3421-04	1.904	0.0	0.008	
L3421-05	1.946	0.0	0.008	
L3421-06	1.493	0.0	0.008	
L3421-07	1.723	0.0	0.008	
L3442-01	1.842	0.0	0.008	
L3442-02	1.769	0.0	0.008	
L3514-02	1.398	0.0	0.008	
L3514-03	1.527	0.0	0.008	
L3514-06	1.992	0.0	0.008	
L3514-07	1.086	0.0	0.008	
L3514-08	2.037	0.0	0.008	
L3514-16	1.920	0.0	0.008	
L3514-17	92.709	0.0	0.102	
CCV002 CCV002	241.609	0.0	0.255	
CCB002 CCB002	1.661	0.0	0.008	

N	22
Mean	31.956
SD	73.2748
CV%	229.30

Aquakem v. 7.2AQ1

Results from time period:

Fri Jul 31 16:49:21 2020

Fri Jul 31 17:37:43 2020

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time
S0.0	A	CNEPA-NE\ P		0.344	µg/l	7/31/2020 16:49:21
S5.0	A	CNEPA-NE\ P		5.5436	µg/l	7/31/2020 16:49:22
S10.0	A	CNEPA-NE\ P		10.6852	µg/l	7/31/2020 16:49:23
S100.0	A	CNEPA-NE\ P		98.8055	µg/l	7/31/2020 16:49:24
S250.0	A	CNEPA-NE\ P		248.8038	µg/l	7/31/2020 16:49:25
S500.0	A	CNEPA-NE\ P		500.8178	µg/l	7/31/2020 16:49:26
ICV ICV	S	CNEPA-NE\ P		95.4967	µg/l	7/31/2020 17:29:58
ICB ICB	S	CNEPA-NE\ P		1.2383	µg/l	7/31/2020 17:29:59
CCV001 CCV001	S	CNEPA-NE\ P		243.0582	µg/l	7/31/2020 17:30:00
CCB001 CCB001	S	CNEPA-NE\ P		1.3798	µg/l	7/31/2020 17:30:01
PB130566BL PBW566	S	CNEPA-NE\ P		1.0698	µg/l	7/31/2020 17:30:02
L3421-02	S	CNEPA-NE\ P		1.7134	µg/l	7/31/2020 17:30:03
L3421-03	S	CNEPA-NE\ P		2.4628	µg/l	7/31/2020 17:30:04
L3421-04	S	CNEPA-NE\ P		1.9039	µg/l	7/31/2020 17:30:05
L3421-05	S	CNEPA-NE\ P		1.9459	µg/l	7/31/2020 17:30:06
L3421-06	S	CNEPA-NE\ P		1.4928	µg/l	7/31/2020 17:30:07
L3421-07	S	CNEPA-NE\ P		1.7229	µg/l	7/31/2020 17:30:08
L3442-01	S	CNEPA-NE\ P		1.842	µg/l	7/31/2020 17:37:33
L3442-02	S	CNEPA-NE\ P		1.7693	µg/l	7/31/2020 17:37:34
L3514-02	S	CNEPA-NE\ P		1.3978	µg/l	7/31/2020 17:37:35
L3514-03	S	CNEPA-NE\ P		1.5268	µg/l	7/31/2020 17:37:36
L3514-06	S	CNEPA-NE\ P		1.9919	µg/l	7/31/2020 17:37:37
L3514-07	S	CNEPA-NE\ P		1.0859	µg/l	7/31/2020 17:37:38
L3514-08	S	CNEPA-NE\ P		2.0371	µg/l	7/31/2020 17:37:39
L3514-16	S	CNEPA-NE\ P		1.9201	µg/l	7/31/2020 17:37:40
L3514-17	S	CNEPA-NE\ P		92.7093	µg/l	7/31/2020 17:37:41
CCV002 CCV002	S	CNEPA-NE\ P		241.6087	µg/l	7/31/2020 17:37:42
CCB002 CCB002	S	CNEPA-NE\ P		1.6613	µg/l	7/31/2020 17:37:43

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : Am

Instrument ID : Konelab

7/31/2020 16:49


Test CNEPA-NEW

Accepted 7/31/2020 16:49

Factor 973.7
 Bias 0.006

Coeff. of det. 0.999978

Errors

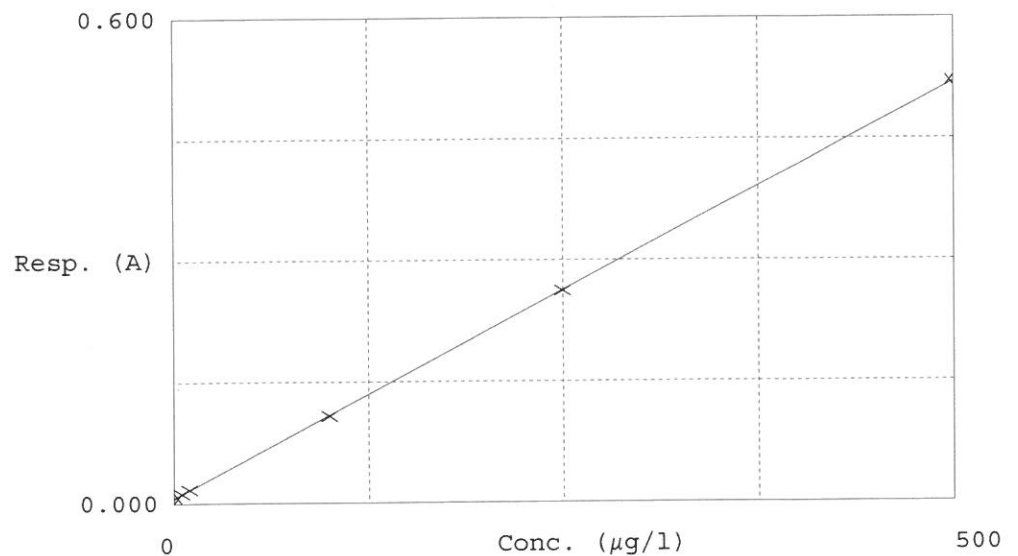

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.007	0.3440	0.0000	
2	5.0PPBCN	0.012	5.5436	5.0000	
3	10PPBCN	0.017	10.6852	10.0000	
4	100PPBCN	0.108	98.8055	100.0000	
5	250PPBCN	0.262	248.8038	250.0000	
6	500PPBCN	0.521	500.8178	500.0000	