

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AM

Instrument ID : Konelab

8/3/2020 13:23


Test Total CN

Accepted 8/3/2020 13:23

Factor 1291
Bias 0.001

Coeff. of det. 0.999976

Errors

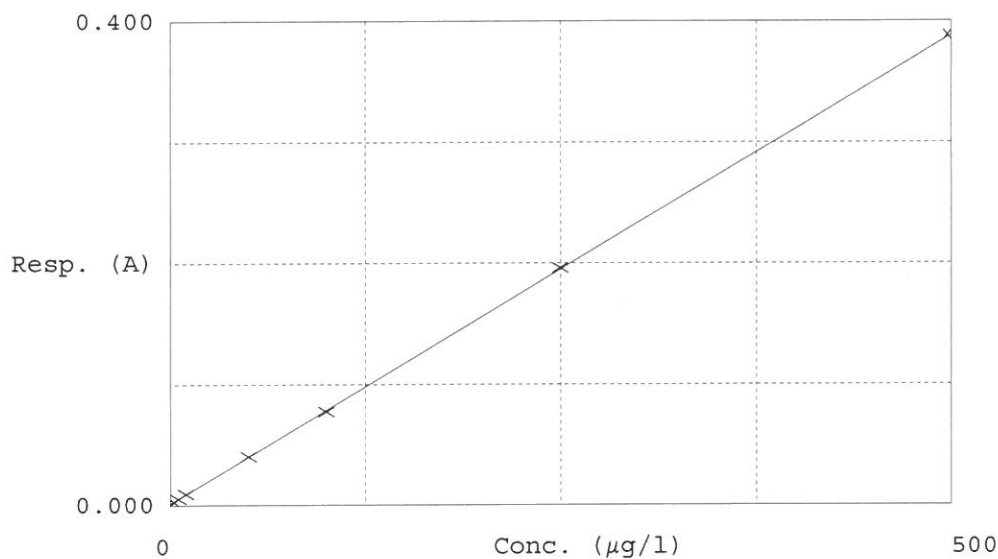

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	-0.1236	0.0000	
2	5.0PPBCN	0.005	5.3143	5.0000	
3	10PPBCN	0.009	10.3557	10.0000	
4	50PPBCN	0.040	50.1798	50.0000	
5	100PPBCN	0.077	98.3063	100.0000	
6	250PPBCN	0.196	251.3140	250.0000	
7	500PPBCN	0.388	499.6535	500.0000	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092

Reviewed by : _____

Instrument ID : Konelab

8/3/2020 14:28

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.471	0.0	0.075	
ICB1	0.673	0.0	0.002	
CCV1	244.045	0.0	0.190	
CCB1	0.497	0.0	0.002	
L3483-02	0.472	0.0	0.002	
PB130664BL	0.435	0.0	0.002	
L3507-07	0.636	0.0	0.002	
L3507-07DUP	0.601	0.0	0.002	
L3511-03	0.569	0.0	0.002	
L3511-08	0.452	0.0	0.002	
L3511-13	0.927	0.0	0.002	
L3511-18	0.278	0.0	0.002	
L3518-03	0.381	0.0	0.002	
L3518-08	0.729	0.0	0.002	
CCV2	245.272	0.0	0.191	
CCB2	0.561	0.0	0.002	
L3518-13	0.706	0.0	0.002	
L3518-18	1.751	0.0	0.003	
L3518-23	0.503	0.0	0.002	
L3518-28	0.275	0.0	0.002	
L3518-33	0.309	0.0	0.002	
L3518-38	0.437	0.0	0.002	
L3518-43	0.242	0.0	0.002	
L3518-48	0.352	0.0	0.002	
PB130696BL	0.417	0.0	0.002	
L3537-04	0.627	0.0	0.002	
CCV3	247.903	0.0	0.193	
CCB3	0.481	0.0	0.002	
L3537-04DUP	0.409	0.0	0.002	
PB130697BL	0.182	0.0	0.002	
L3521-04	0.227	0.0	0.002	
L3521-04DUP	0.277	0.0	0.002	
L3521-08	0.049	0.0	0.001	
L3537-01	0.356	0.0	0.002	
L3537-02	0.530	0.0	0.002	
L3537-03	0.291	0.0	0.002	
CCV4	250.416	0.0	0.195	
CCB4	0.576	0.0	0.002	

N	38
Mean	28.929
SD	77.3205
CV%	267.27

Aquakem v. 7.2AQ1

Results from time period:

Mon Aug 03 13:19:23 2020

Mon Aug 03 14:28:03 2020

Sample Id	Sam/Ctr/cAl	Test short Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive Cl P	-0.1236	µg/l	8/3/2020 13:19:23	
5.OPPBCN	A	Reactive Cl P	5.3143	µg/l	8/3/2020 13:19:24	
10PPBCN	A	Reactive Cl P	10.3557	µg/l	8/3/2020 13:19:25	
50PPBCN	A	Reactive Cl P	50.1798	µg/l	8/3/2020 13:19:26	
100PPBCN	A	Reactive Cl P	98.3063	µg/l	8/3/2020 13:19:27	
250PPBCN	A	Reactive Cl P	251.314	µg/l	8/3/2020 13:19:28	
500PPBCN	A	Reactive Cl P	499.6535	µg/l	8/3/2020 13:19:29	
ICV1	S	Reactive Cl P	95.4715	µg/l	8/3/2020 14:08:05	
ICB1	S	Reactive Cl P	0.6729	µg/l	8/3/2020 14:08:06	
CCV1	S	Reactive Cl P	244.0454	µg/l	8/3/2020 14:08:07	
CCB1	S	Reactive Cl P	0.4968	µg/l	8/3/2020 14:08:08	
L3483-02	S	Reactive Cl P	0.472	µg/l	8/3/2020 14:08:09	
PB130664BL	S	Reactive Cl P	0.4347	µg/l	8/3/2020 14:08:10	
L3507-07	S	Reactive Cl P	0.6359	µg/l	8/3/2020 14:08:11	
L3507-07DUP	S	Reactive Cl P	0.6015	µg/l	8/3/2020 14:08:12	
L3511-03	S	Reactive Cl P	0.5691	µg/l	8/3/2020 14:08:13	
L3511-08	S	Reactive Cl P	0.4517	µg/l	8/3/2020 14:08:14	
L3511-13	S	Reactive Cl P	0.9275	µg/l	8/3/2020 14:08:15	
L3511-18	S	Reactive Cl P	0.2776	µg/l	8/3/2020 14:15:37	
L3518-03	S	Reactive Cl P	0.3813	µg/l	8/3/2020 14:15:38	
L3518-08	S	Reactive Cl P	0.7294	µg/l	8/3/2020 14:15:39	
CCV2	S	Reactive Cl P	245.272	µg/l	8/3/2020 14:15:40	
CCB2	S	Reactive Cl P	0.5609	µg/l	8/3/2020 14:15:41	
L3518-13	S	Reactive Cl P	0.7058	µg/l	8/3/2020 14:15:42	
L3518-18	S	Reactive Cl P	1.7508	µg/l	8/3/2020 14:15:43	
L3518-23	S	Reactive Cl P	0.5032	µg/l	8/3/2020 14:15:44	
L3518-28	S	Reactive Cl P	0.2746	µg/l	8/3/2020 14:15:45	
L3518-33	S	Reactive Cl P	0.3089	µg/l	8/3/2020 14:15:46	
L3518-38	S	Reactive Cl P	0.4368	µg/l	8/3/2020 14:15:47	
L3518-43	S	Reactive Cl P	0.2416	µg/l	8/3/2020 14:23:12	
L3518-48	S	Reactive Cl P	0.3525	µg/l	8/3/2020 14:23:13	
PB130696BL	S	Reactive Cl P	0.4172	µg/l	8/3/2020 14:23:14	
L3537-04	S	Reactive Cl P	0.6271	µg/l	8/3/2020 14:23:15	
CCV3	S	Reactive Cl P	247.9027	µg/l	8/3/2020 14:23:16	
CCB3	S	Reactive Cl P	0.4814	µg/l	8/3/2020 14:23:17	
L3537-04DUP	S	Reactive Cl P	0.4088	µg/l	8/3/2020 14:23:18	
PB130697BL	S	Reactive Cl P	0.1818	µg/l	8/3/2020 14:23:19	
L3521-04	S	Reactive Cl P	0.2273	µg/l	8/3/2020 14:23:20	
L3521-04DUP	S	Reactive Cl P	0.277	µg/l	8/3/2020 14:23:21	
L3521-08	S	Reactive Cl P	0.0486	µg/l	8/3/2020 14:23:22	
L3537-01	S	Reactive Cl P	0.3562	µg/l	8/3/2020 14:27:59	
L3537-02	S	Reactive Cl P	0.5296	µg/l	8/3/2020 14:28:00	

L3537-03	S	Reactive Cl P	0.291 µg/l	8/3/2020 14:28:01
CCV4	S	Reactive Cl P	250.4157 µg/l	8/3/2020 14:28:02
CCB4	S	Reactive Cl P	0.5765 µg/l	8/3/2020 14:28:03