

LB110394

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AM

Instrument ID : Konelab

8/6/2020 10:27

Test: Total CN

Sample Id	Result ^{ug/L}	Dil. 1 +	Response	Errors
CCV1	253.243	0.0	0.203	
CCB1	0.284	0.0	0.003	
PB130732BL	0.161	0.0	0.003	
L3545-01	0.193	0.0	0.003	
L3545-01DUP	0.112	0.0	0.003	
L3547-02	0.171	0.0	0.003	
L3548-02	0.214	0.0	0.003	
L3548-05	0.025	0.0	0.003	
L3548-08	0.092	0.0	0.003	
L3548-11	-0.122	0.0	0.003	
L3553-04	0.326	0.0	0.003	
L3502-05	0.636	0.0	0.004	
CCV2	263.693	0.0	0.211	
CCB2	0.203	0.0	0.003	

N	14
Mean	37.088
SD	93.8122
CV%	252.95

Aquakem v. 7.2AQ1

Results from time period:

Thu Aug 06 10:22:28 2020

Thu Aug 06 10:27:19 2020

Sample Id	Sam/Ctr/c/	Test short name	Test type	Result	Result unit	Result date and tim	Stat
0.0PPBCN	A	Reactive CN	P	-0.6152	µg/l	8/6/2020 8:32:27	
5.0PPBCN	A	Reactive CN	P	4.6777	µg/l	8/6/2020 8:32:28	
10PPBCN	A	Reactive CN	P	9.7513	µg/l	8/6/2020 8:32:29	
50PPBCN	A	Reactive CN	P	50.0497	µg/l	8/6/2020 8:32:30	
100PPBCN	A	Reactive CN	P	100.4635	µg/l	8/6/2020 8:32:31	
250PPBCN	A	Reactive CN	P	251.5251	µg/l	8/6/2020 8:32:32	
500PPBCN	A	Reactive CN	P	499.148	µg/l	8/6/2020 8:32:33	
ICV1	S	Reactive CN	P	96.0383	µg/l	8/6/2020 9:15:51	
ICB1	S	Reactive CN	P	0.3559	µg/l	8/6/2020 9:15:52	
CCV1	S	Reactive CN	P	253.2427	µg/l	8/6/2020 10:22:30	
CCB1	S	Reactive CN	P	0.2837	µg/l	8/6/2020 10:22:31	
PB130732BL	S	Reactive CN	P	0.1608	µg/l	8/6/2020 10:22:32	
L3545-01	S	Reactive CN	P	0.1926	µg/l	8/6/2020 10:22:33	
L3545-01DUP	S	Reactive CN	P	0.1125	µg/l	8/6/2020 10:22:34	
L3547-02	S	Reactive CN	P	0.1708	µg/l	8/6/2020 10:22:35	
L3548-02	S	Reactive CN	P	0.2144	µg/l	8/6/2020 10:22:36	
L3548-05	S	Reactive CN	P	0.0248	µg/l	8/6/2020 10:22:37	
L3548-08	S	Reactive CN	P	0.0918	µg/l	8/6/2020 10:22:38	
L3548-11	S	Reactive CN	P	-0.1218	µg/l	8/6/2020 10:27:15	
L3553-04	S	Reactive CN	P	0.326	µg/l	8/6/2020 10:27:16	
L3502-05	S	Reactive CN	P	0.6364	µg/l	8/6/2020 10:27:17	
CCV2	S	Reactive CN	P	263.6931	µg/l	8/6/2020 10:27:18	
CCB2	S	Reactive CN	P	0.2033	µg/l	8/6/2020 10:27:19	

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : AM

Instrument ID : Konelab

8/6/2020 8:33


Test Total CN

Accepted 8/6/2020 8:32

Factor 1268
 Bias 0.003

Coeff. of det. 0.999981

Errors

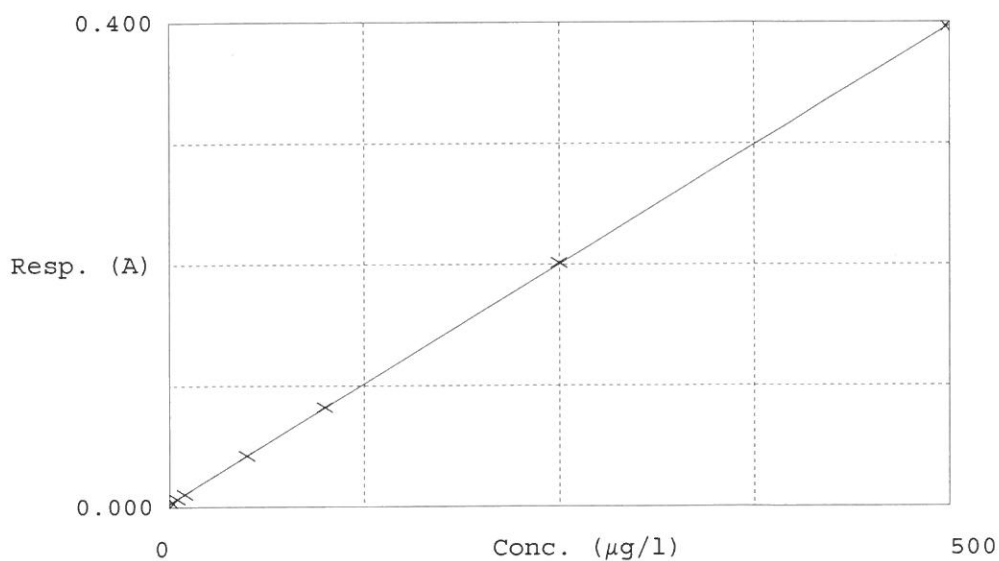

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-0.6152	0.0000	
2	5.0PPBCN	0.007	4.6777	5.0000	
3	10PPBCN	0.011	9.7513	10.0000	
4	50PPBCN	0.043	50.0497	50.0000	
5	100PPBCN	0.082	100.4635	100.0000	
6	250PPBCN	0.201	251.5251	250.0000	
7	500PPBCN	0.397	499.1480	500.0000	