

Clear table


ident	concentra tion F-	concentrati on CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final Vol	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2020-07-14_	7/14/20 10:45		AM/AP
STD2	0.2310	0.3700	0.3650	1.2140	0.3120	0.0150	1.8910	0.0000_2020-07-14_	7/14/20 11:18		AM/AP
STD3	0.3820	0.6370	0.6330	2.1460	0.5370	0.6980	3.1650	0.0000_2020-07-14_	7/14/20 11:51		AM/AP
STD4	0.8580	1.2490	1.2330	4.0910	1.0320	0.8410	6.0620	0.0000_2020-07-14_	7/14/20 12:23		AM/AP
STD5	1.9540	3.0150	3.0120	10.0090	2.4850	4.3990	14.4120	0.0000_2020-07-14_	7/14/20 12:56		AM/AP
STD6	3.9330	6.1140	6.1220	20.3480	5.0720	8.8220	29.7130	0.0000_2020-07-14_	7/14/20 13:29		AM/AP
STD7	5.0850	7.5430	7.5440	25.1290	6.2940	12.4760	37.8110	0.0000_2020-07-14_	7/14/20 14:01		AM/AP
ICV	2.0840	2.8560	2.8560	9.4580	2.3620	4.5040	14.1500	0.0000_2020-07-14_	7/14/20 15:22		AM/AP
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2020-07-14_	7/14/20 16:00		AM/AP
CCV	1.9990	2.8610	2.8940	9.6110	2.3970	5.4860	13.8870	0.0000_2020-08-07_	8/7/20 9:24		AM/AP
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2020-08-07_	8/7/20 10:01		AM/AP
LB110423BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2020-08-07_	8/7/20 10:32		AM/AP
LB110423BSW	2.0020	2.8500	2.8880	9.6190	2.4010	5.6280	13.8260	0.0000_2020-08-07_	8/7/20 11:02		AM/AP
L3605-01	0.7430	12.4920	0.0000	0.0000	0.1280	1.1970	3.6020	0.0000_2020-08-07_	8/7/20 12:12		AM/AP
L3605-01DUP	0.7190	12.5050	0.0000	0.0000	0.1300	1.1660	3.6300	0.0000_2020-08-07_	8/7/20 12:43		AM/AP
L3605-01MS	2.6370	14.6130	2.8390	9.6320	2.4700	7.8910	16.9560	0.0000_2020-08-07_	8/7/20 13:13		AM/AP
L3605-01MSD	2.6010	14.6000	2.8260	9.5980	2.4520	7.9250	16.8770	0.0000_2020-08-07_	8/7/20 13:44		AM/AP
L3605-01DLX3	0.3090	3.7930	0.0000	0.0000	0.0900	0.2780	1.4070	0.0000_2020-08-07_	8/7/20 14:15		AM/AP
CCV	1.9380	2.7640	2.7960	9.3370	2.3340	5.6650	13.5750	0.0000_2020-08-07_	8/7/20 14:57		AM/AP
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2020-08-07_	8/7/20 15:29		AM/AP
L3621-01	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2020-08-07_	8/7/20 16:01		AM/AP
L3621-02	0.0000	0.1060	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2020-08-07_	8/7/20 16:32		AM/AP
L3621-03	0.0000	0.0000	0.0000	0.0000	0.0800	0.0000	0.0000	0.0000_2020-08-07_	8/7/20 17:04		AM/AP
CCV	1.8910	2.7470	2.7830	9.3170	2.3270	5.4730	13.5360	0.0000_2020-08-07_	8/7/20 17:36		AM/AP
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000_2020-08-07_	8/7/20 18:07		AM/AP

IC-2
300.0
8/10/2020
Am

CALIBRATION OF COMPONENT F-

Method: AnionsIC2-071420.mtw
 Equation: $Q = 0.0763439 \cdot A + 2.139$
 RSD: 3.690 %
 Correlation coefficient: 0.999425

IC-2
 300.0
 8/10/2020
 AM

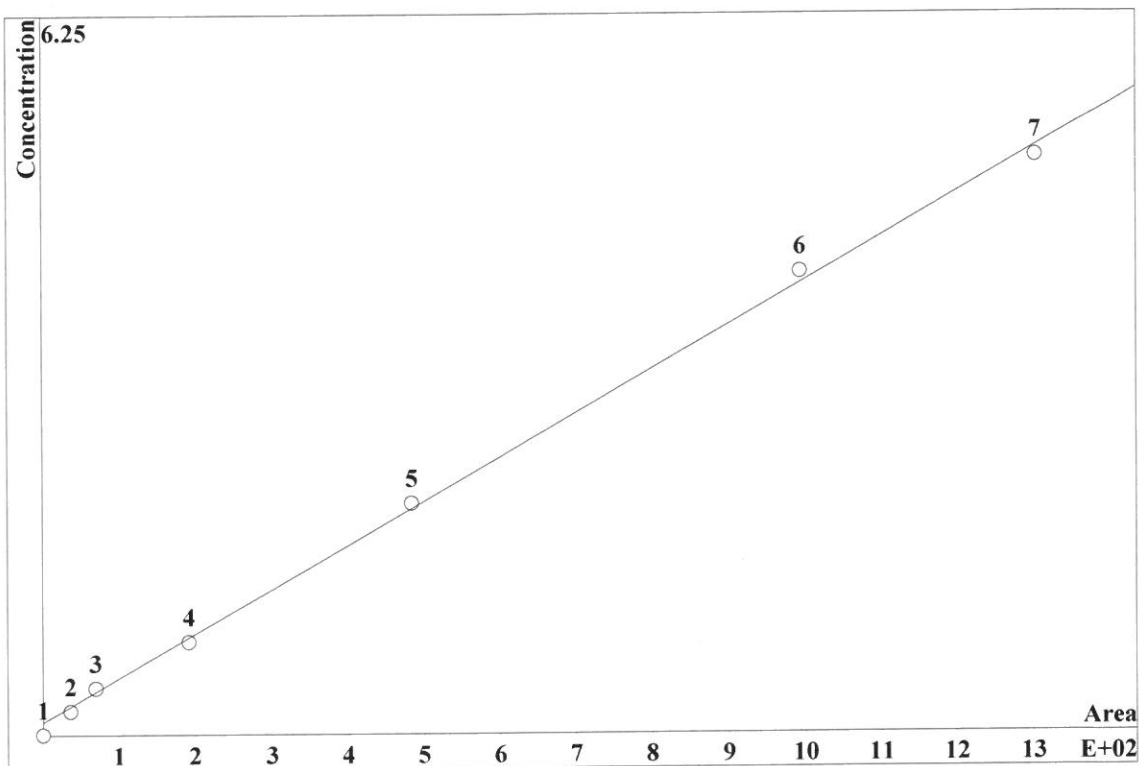


K3 = 0 K2 = 0 K1 = 0.0763439 K0 = 2.139
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	1.713	36.03	0.2	20	5.75		
3	3.346	69.49	0.4	20	5.75		
4	8.712	192.2	0.8	20	5.75		
5	24.16	484.1	2	20	5.75		
6	50.68	994.3	4	20	5.75		
7	70.95	1304	5	20	5.75		

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-071420.mtw
 Equation: $Q = 0.119172 \cdot A + 1.16617$
 RSD: 1.675 %
 Correlation coefficient: 0.999881

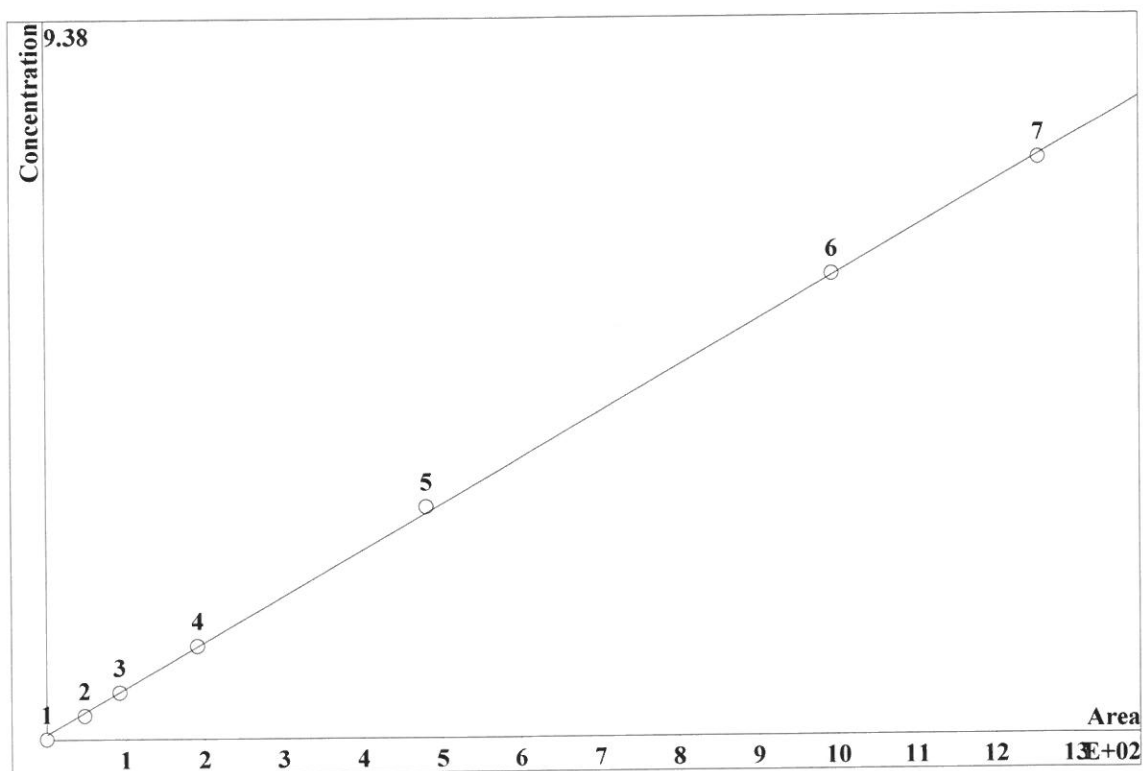


K3 = 0 K2 = 0 K1 = 0.119172 K0 = 1.16617
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	2.952	48.41	0.3	20	8.834		
3	5.72	92.8	0.6	20	8.834		
4	11.68	191.1	1.2	20	8.834		
5	30.26	480.4	3	20	8.834		
6	64.4	994	6	20	8.834		
7	81.81	1256	7.5	20	8.834		

CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-071420.mtw
 Equation: $Q = 0.051754 \cdot A + 1.61453$
 RSD: 1.829 %
 Correlation coefficient: 0.999859

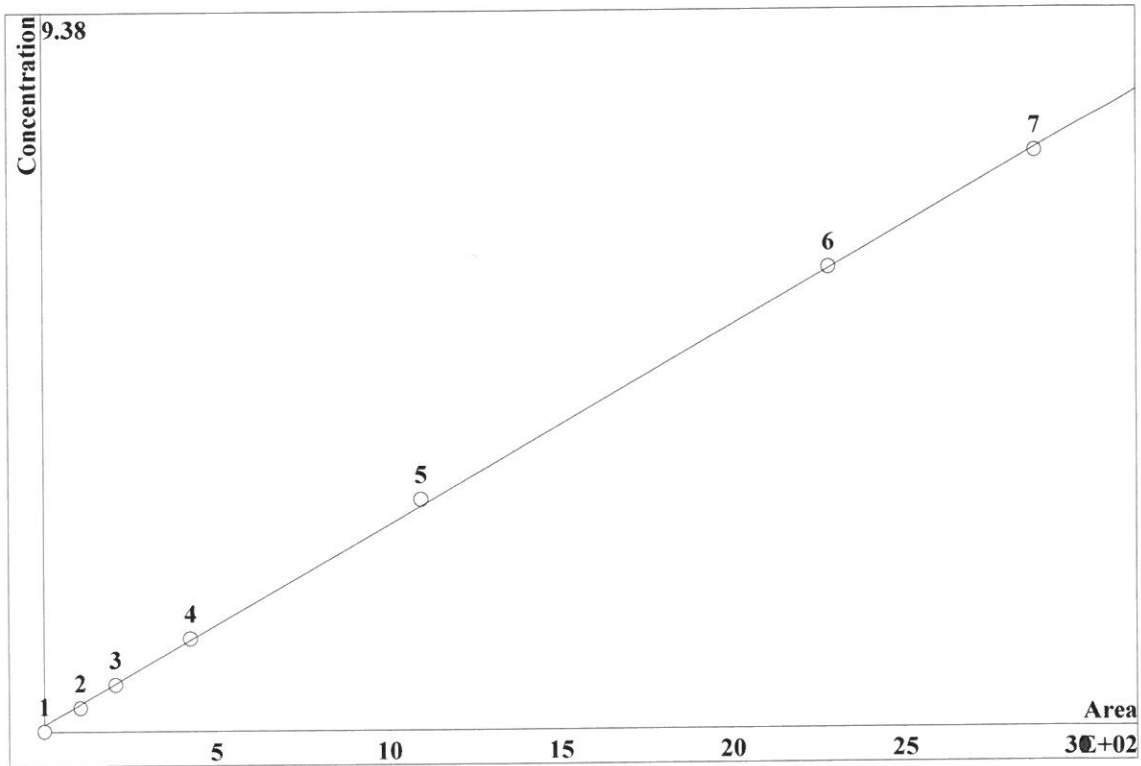


K3 = 0 K2 = 0 K1 = 0.051754 K0 = 1.61453
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	5.227	105.7	0.3	20	10.64		
3	10.22	207.7	0.6	20	10.64		
4	20.98	426.5	1.2	20	10.64		
5	54.22	1095	3	20	10.64		
6	110	2281	6	20	10.64		
7	139.3	2884	7.5	20	10.64		

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-071420.mtw
 Equation: $Q = 0.267495 \cdot A + 5.42473$
 RSD: 1.764 %
 Correlation coefficient: 0.999869

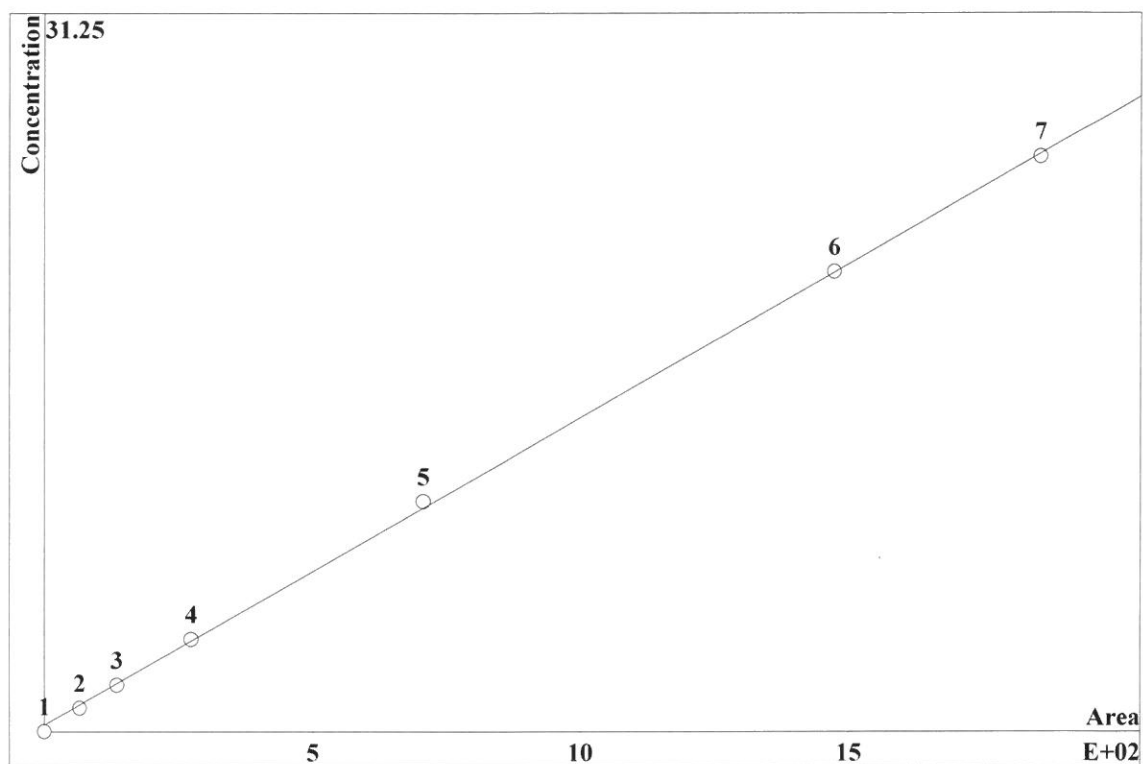

K3 = 0 K2 = 0 K1 = 0.267495 K0 = 5.42473

Base: Area

Ref.channel: chl

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	2.914	66.1	1	20			14
3	5.879	136.1	2	20			14
4	12.2	274.1	4	20			14
5	32.27	706.4	10	20			14
6	69.57	1473	20	20			14
7	88.74	1859	25	20			14

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-071420.mtw
 Equation: $Q = 0.0472497 \cdot A + 1.18063$
 RSD: 2.042 %
 Correlation coefficient: 0.999824

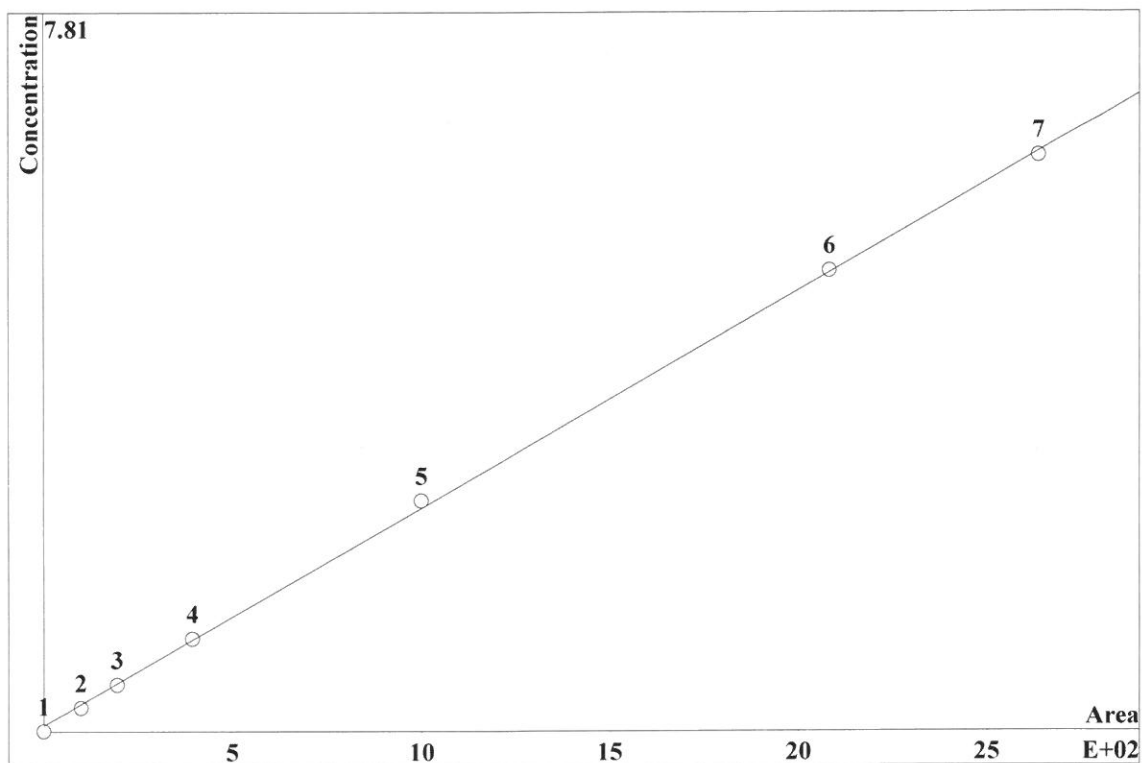

K3 = 0 K2 = 0 K1 = 0.0472497 K0 = 1.18063

Base: Area

Ref.channel: chl

ISTD:

Formula: Linear


Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	3.509	99.57	0.25	20	16.26		
3	6.967	194.8	0.5	20	16.26		
4	14.26	395	1	20	16.26		
5	36.99	999.4	2.5	20	16.26		
6	79.04	2083	5	20	16.26		
7	101.1	2639	6.25	20	16.26		

20□

CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-071420.mtw
 Equation: $Q = 0.106077 \cdot A - 8.7791$
 RSD: 1.905 %
 Correlation coefficient: 0.999847

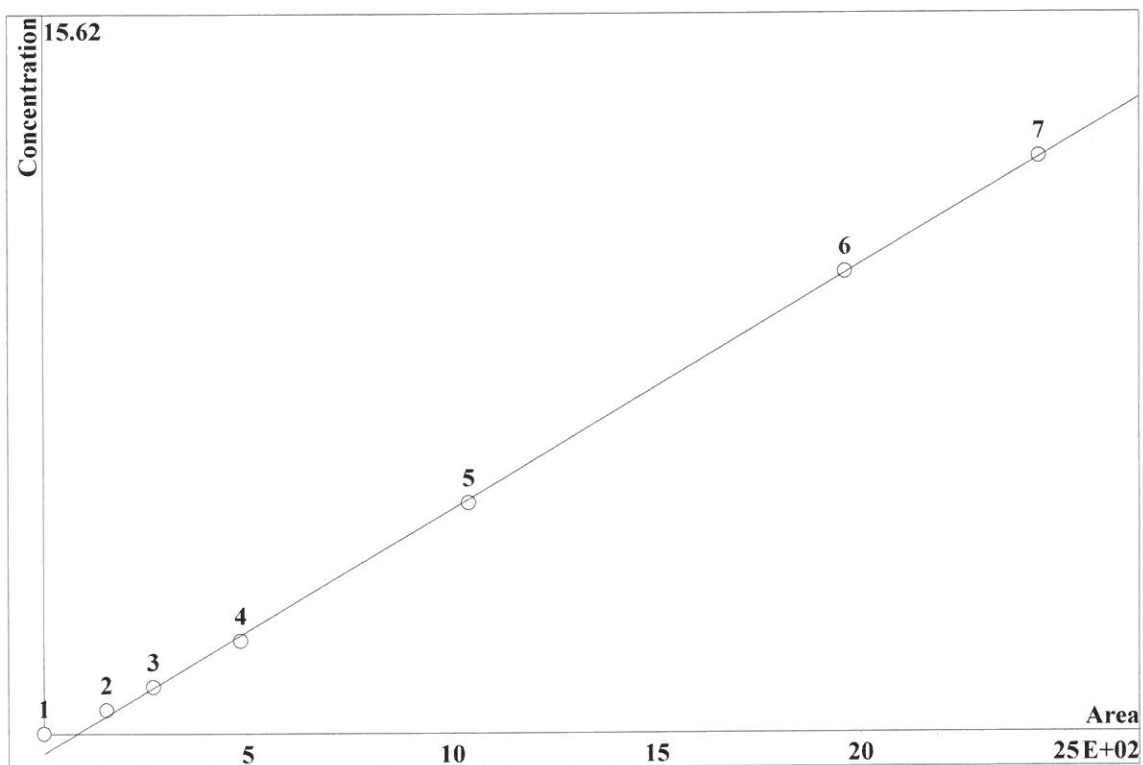

K3 = 0 K2 = 0 K1 = 0.106077 K0 = -8.7791

Base: Area

Ref.channel: chl

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	3.468	152.8	0.5	20	21.2		
3	6.287	268.2	1	20	21.2		
4	11.66	482.6	2	20	21.2		
5	26.07	1040	5	20	21.2		
6	51.11	1963	10	20	21.2		
7	64.03	2435	12.5	20	21.2		

CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-071420.mtw
 Equation: $Q = 0.161568 \cdot A + 8.56697$
 RSD: 2.425 %
 Correlation coefficient: 0.999751

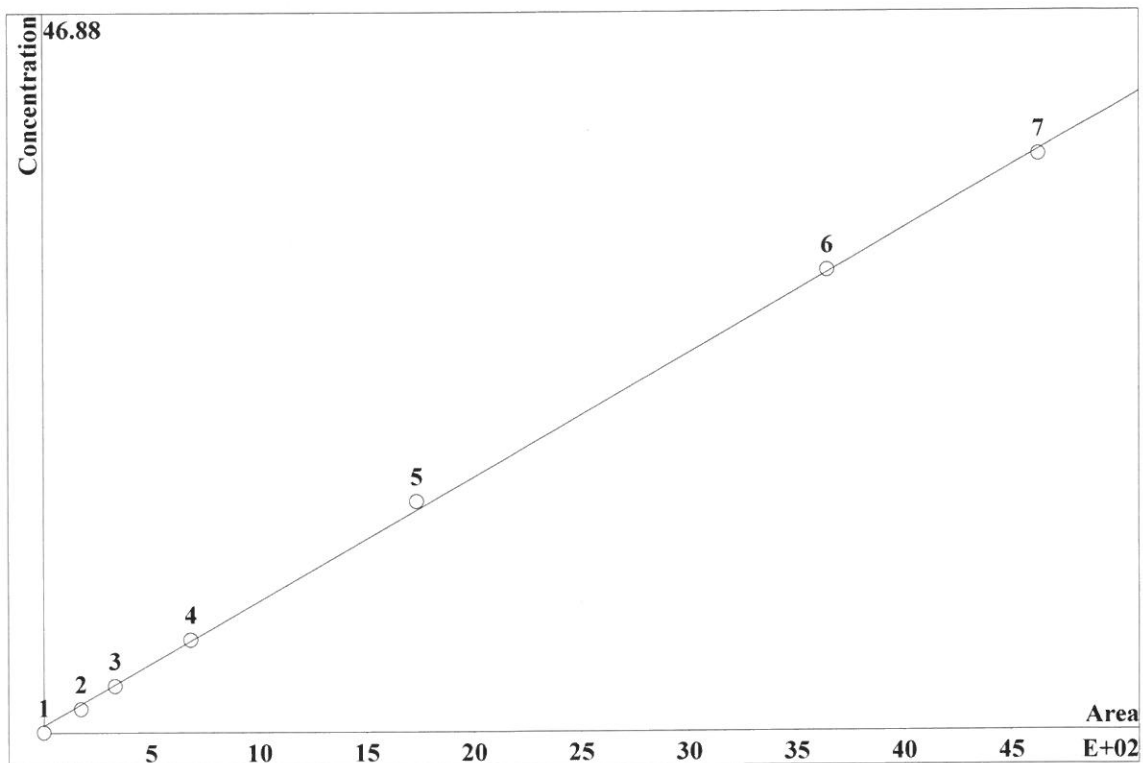

K3 = 0 K2 = 0 K1 = 0.161568 K0 = 8.56697

Base: Area

Ref.channel: chl

ISTD:

Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	4.775	173.6	1.5	20	24.73		
3	9.183	332.7	3	20	24.73		
4	18.7	683.8	6	20	24.73		
5	47.94	1733	15	20	24.73		
6	102.4	3643	30	20	24.73		
7	130.1	4628	37.5	20	24.73		

Report date: 8/10/2020 9:31:20 AM
Printed by: wet

Ident: STD1
Analysis from: 7/14/2020 10:45:51 AM
File: _2020-07-14_


Last save: 7/14/2020 11:15:49 AM

Method: AnionsIC2-071420.mtw
Run operator: wet
Analysis number: 26538

Last save: 7/14/2020 9:36:

SAMPLE:
: AM/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

IC-2
8/10/2020
300.0
87 AM

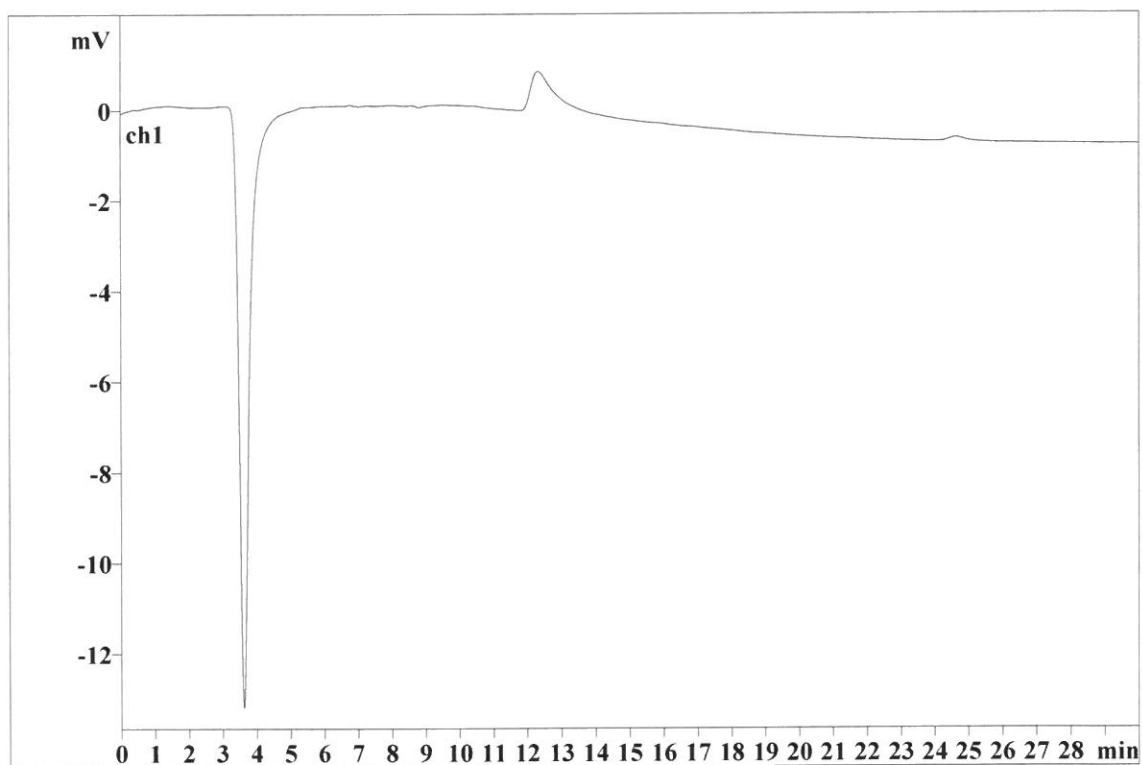

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/10/2020 9:31:27 AM
Printed by: wet


Ident: STD2
Analysis from: 7/14/2020 11:18:27 AM
File: _2020-07-14_

Last save: 7/14/2020 11:48:28 AM

Method: AnionsIC2-071420.mtw
Run operator: wet
Analysis number: 26539

Last save: 7/14/2020 11:15

SAMPLE:
: AM/AP
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

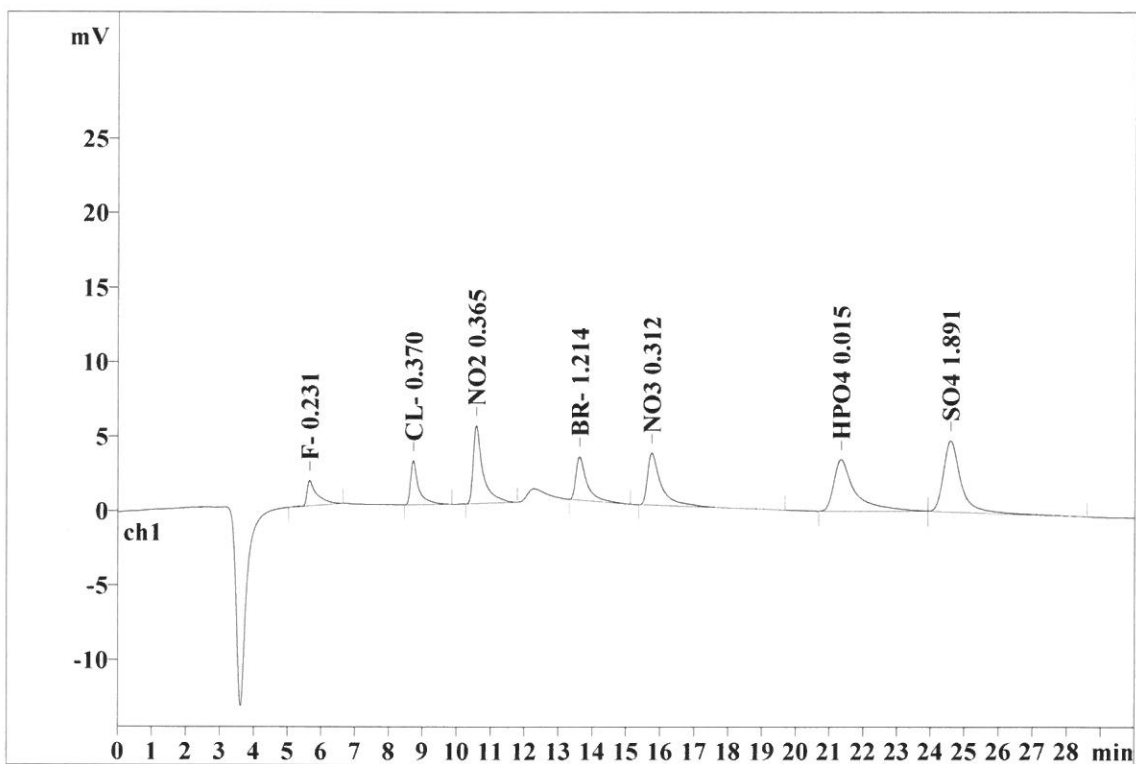

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.64	0.259	1.71	6.97	36.028	5.28
2	8.72	0.205	2.95	12.01	48.411	7.10
3	10.57	0.257	5.23	21.28	105.690	15.49
4	13.62	0.300	2.91	11.86	66.101	9.69
5	15.74	0.362	3.51	14.29	99.566	14.60
6	21.33	0.549	3.47	14.12	152.765	22.39
7	24.58	0.502	4.77	19.44	173.622	25.45
7	30.00	0.348	24.55	99.98	682.184	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/10/2020 9:31:33 AM
Printed by: wet


Ident: STD3
Analysis from: 7/14/2020 11:51:05 AM
File: _2020-07-14_

Last save: 7/14/2020 12:21:06 PM

Method: AnionsIC2-071420.mtw
Run operator: wet
Analysis number: 26540

Last save: 7/14/2020 11:48

SAMPLE:
: AM/AP
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

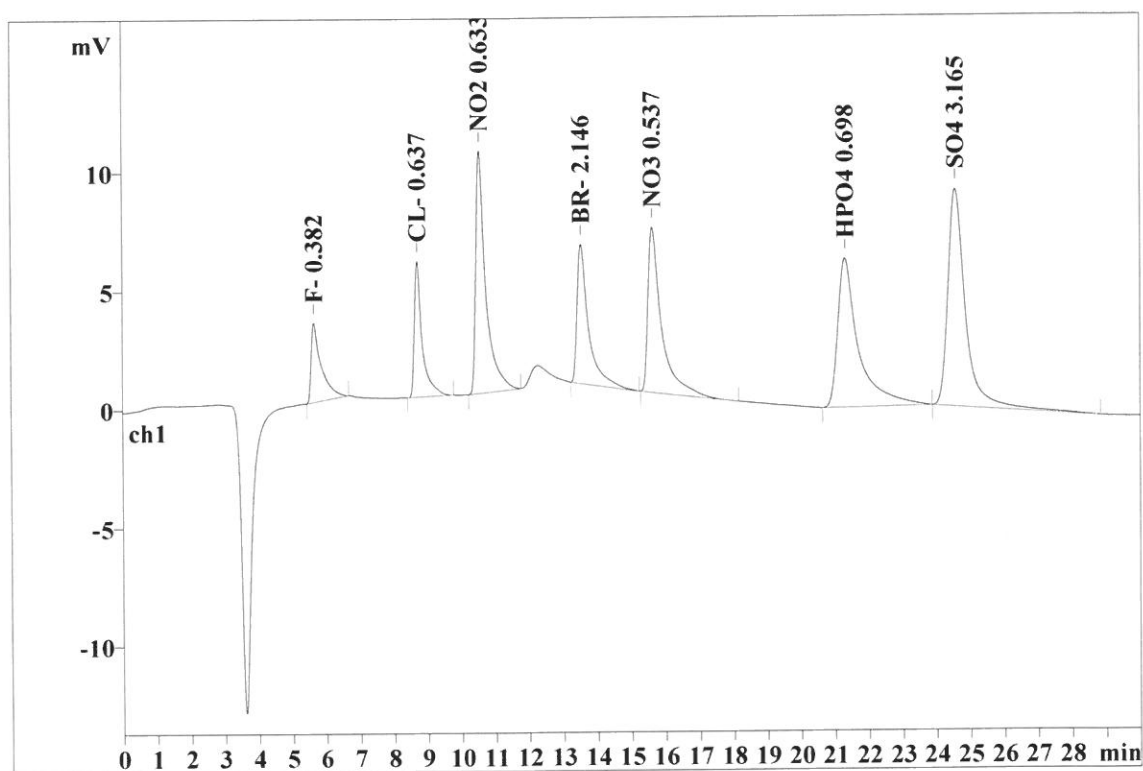

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.64	0.264	3.34	7.03	69.492	5.34
2	8.69	0.205	5.72	12.02	92.797	7.13
3	10.53	0.261	10.22	21.47	207.712	15.96
4	13.54	0.298	5.88	12.35	136.063	10.45
5	15.63	0.358	6.97	14.64	194.816	14.97
6	21.31	0.535	6.29	13.21	268.176	20.60
7	24.58	0.498	9.18	19.29	332.728	25.56
7	30.00	0.346	47.59	99.99	1301.785	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/10/2020 9:31:39 AM
Printed by: wet


Ident: STD4
Analysis from: 7/14/2020 12:23:44 PM
File: _2020-07-14_

Last save: 7/14/2020 12:53:44 PM

Method: AnionsIC2-071420.mtw
Run operator: wet
Analysis number: 26541

Last save: 7/14/2020 12:21

SAMPLE:
: AM/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

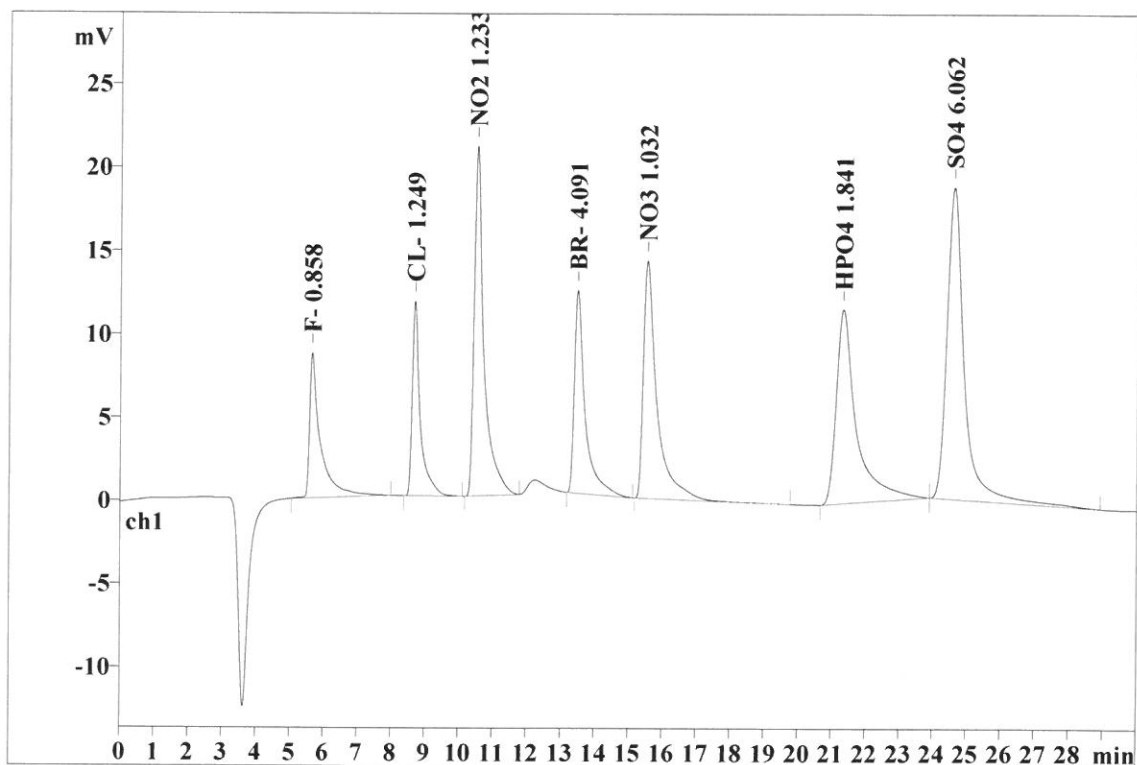

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.65	0.244	8.71	8.87	192.184	7.27
2	8.69	0.205	11.67	11.89	191.096	7.22
3	10.51	0.260	20.98	21.37	426.526	16.12
4	13.48	0.291	12.20	12.42	274.103	10.36
5	15.53	0.354	14.26	14.52	395.012	14.93
6	21.32	0.519	11.66	11.87	482.580	18.24
7	24.61	0.495	18.70	19.05	683.759	25.85
7	30.00	0.338	98.18	100.00	2645.260	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/10/2020 9:31:44 AM
Printed by: wet


Ident: STD5
Analysis from: 7/14/2020 12:56:22 PM
File: _2020-07-14_

Last save: 7/14/2020 1:26:22 PM

Method: AnionsIC2-071420.mtw
Run operator: wet
Analysis number: 26542

Last save: 7/14/2020 12:53

SAMPLE:
: AM/AP
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

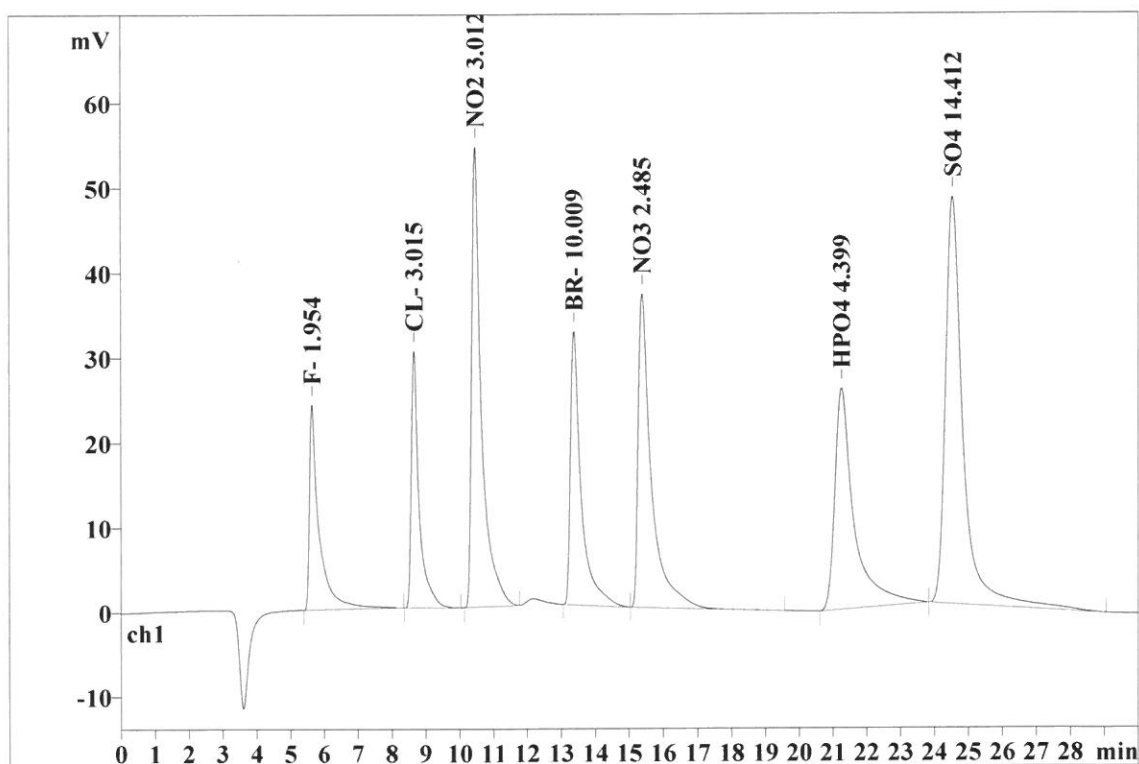

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.63	0.222	24.16	9.59	484.128	7.40
2	8.65	0.199	30.26	12.01	480.392	7.35
3	10.44	0.260	54.22	21.52	1095.369	16.75
4	13.38	0.281	32.27	12.81	706.385	10.80
5	15.37	0.347	36.98	14.68	999.449	15.28
6	21.26	0.503	26.07	10.35	1040.034	15.90
7	24.55	0.486	47.94	19.03	1733.488	26.51
7	30.00	0.328	251.90	99.99	6539.245	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/10/2020 9:31:49 AM
Printed by: wet


Ident: STD6
Analysis from: 7/14/2020 1:29:00 PM
File: _2020-07-14_

Last save: 7/14/2020 1:59:01 PM

Method: AnionsIC2-071420.mtw
Run operator: wet
Analysis number: 26543

Last save: 7/14/2020 1:26:

SAMPLE:
: AM/AP
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

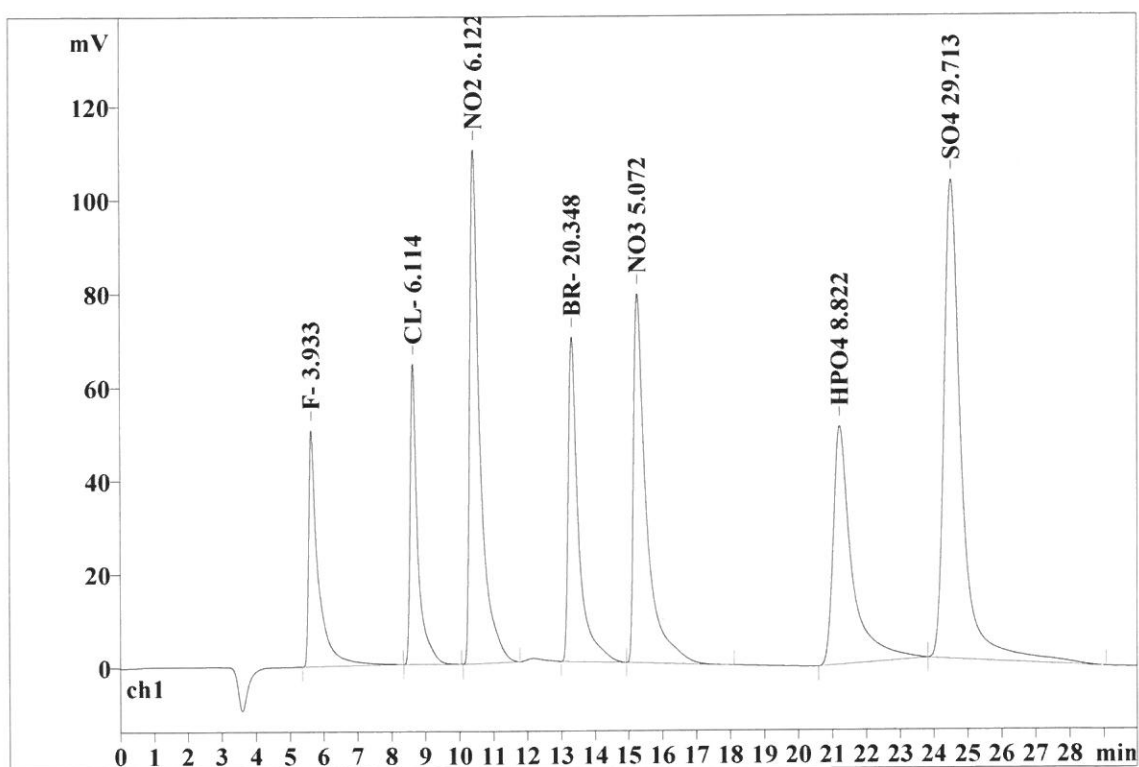

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.64	0.225	50.67	9.61	994.292	7.40
2	8.63	0.195	64.40	12.22	994.027	7.40
3	10.41	0.273	109.99	20.86	2281.353	16.99
4	13.32	0.272	69.57	13.20	1472.740	10.97
5	15.26	0.338	79.03	14.99	2082.840	15.51
6	21.22	0.489	51.11	9.69	1962.776	14.61
7	24.53	0.476	102.43	19.43	3642.933	27.12
7	30.00	0.324	527.21	100.00	13430.961	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/10/2020 9:31:56 AM
Printed by: wet


Ident: STD7
Analysis from: 7/14/2020 2:01:38 PM
File: _2020-07-14_

Last save: 7/14/2020 2:31:38 PM

Method: AnionsIC2-071420.mtw
Run operator: wet
Analysis number: 26544

Last save: 7/14/2020 1:59:

SAMPLE:
: AM/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

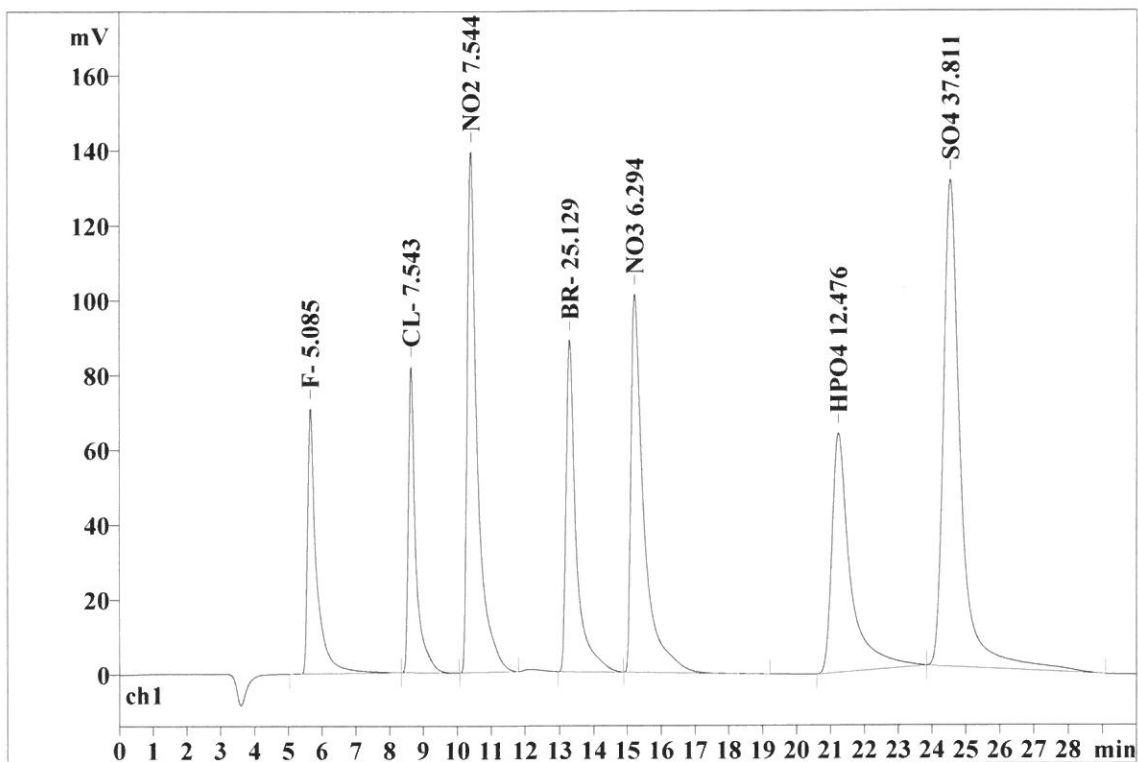

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.65	0.218	70.95	10.49	1304.225	7.67
2	8.63	0.194	81.80	12.10	1256.096	7.39
3	10.38	0.271	139.28	20.60	2884.026	16.96
4	13.30	0.270	88.74	13.13	1858.536	10.93
5	15.21	0.334	101.14	14.96	2639.279	15.52
6	21.23	0.486	64.03	9.47	2435.022	14.32
7	24.55	0.476	130.14	19.25	4627.540	27.21
7	30.00	0.321	676.08	100.00	17004.724	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/10/2020 9:32:06 AM
Printed by: wet


Ident: ICV
Analysis from: 7/14/2020 3:22:46 PM
File: _2020-07-14_

Last save: 7/14/2020 3:52:47 PM

Method: AnionsIC2-071420.mtw
Run operator: wet
Analysis number: 26548

Last save: 7/14/2020 2:31:

SAMPLE:
: AM/AP
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

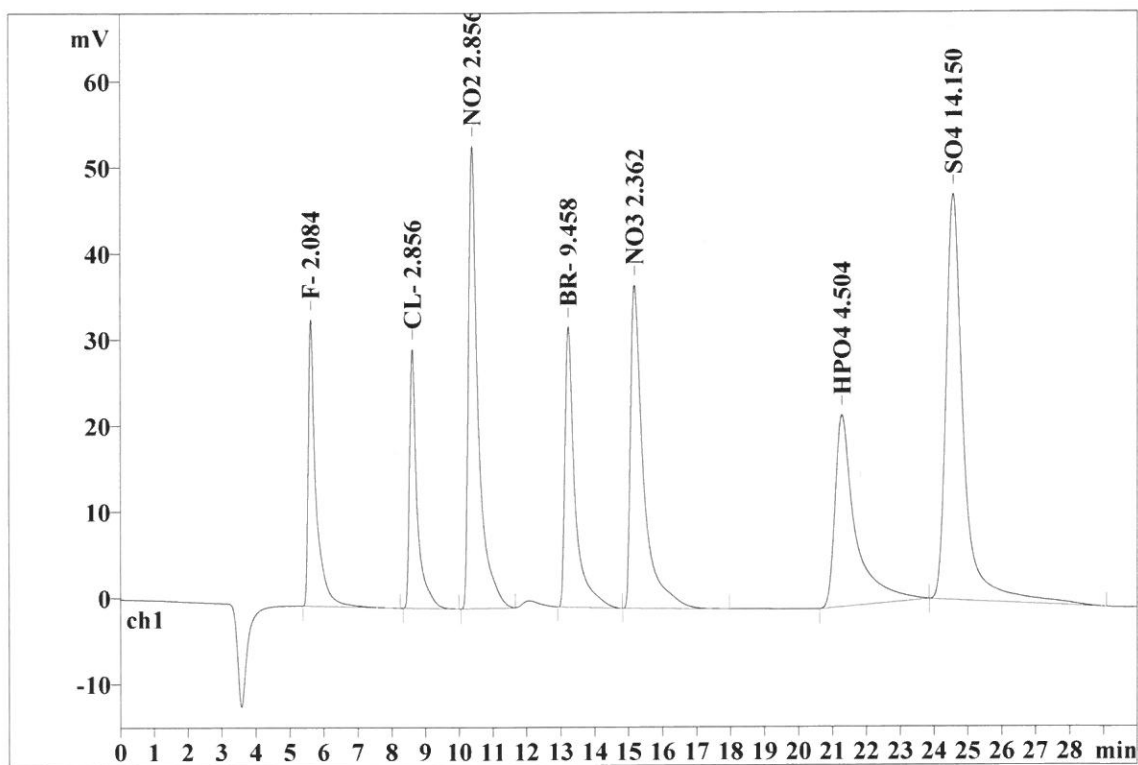

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.61	0.186	33.30	12.97	518.014	8.15
2	8.60	0.198	30.12	11.73	469.449	7.39
3	10.36	0.260	53.77	20.94	1072.567	16.88
4	13.22	0.272	32.57	12.69	686.838	10.81
5	15.17	0.334	37.57	14.64	974.994	15.35
6	21.27	0.519	22.29	8.68	931.878	14.67
7	24.57	0.482	47.12	18.35	1698.533	26.74
7	30.00	0.322	256.73	100.00	6352.272	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/10/2020 9:32:14 AM
Printed by: wet


Ident: ICB
Analysis from: 7/14/2020 4:00:06 PM
File: _2020-07-14_

Last save: 7/14/2020 4:30:06 PM

Method: AnionsIC2-071420.mtw
Run operator: wet
Analysis number: 26549

Last save: 7/14/2020 2:31:

SAMPLE:
: AM/AP
Vial number: 10
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

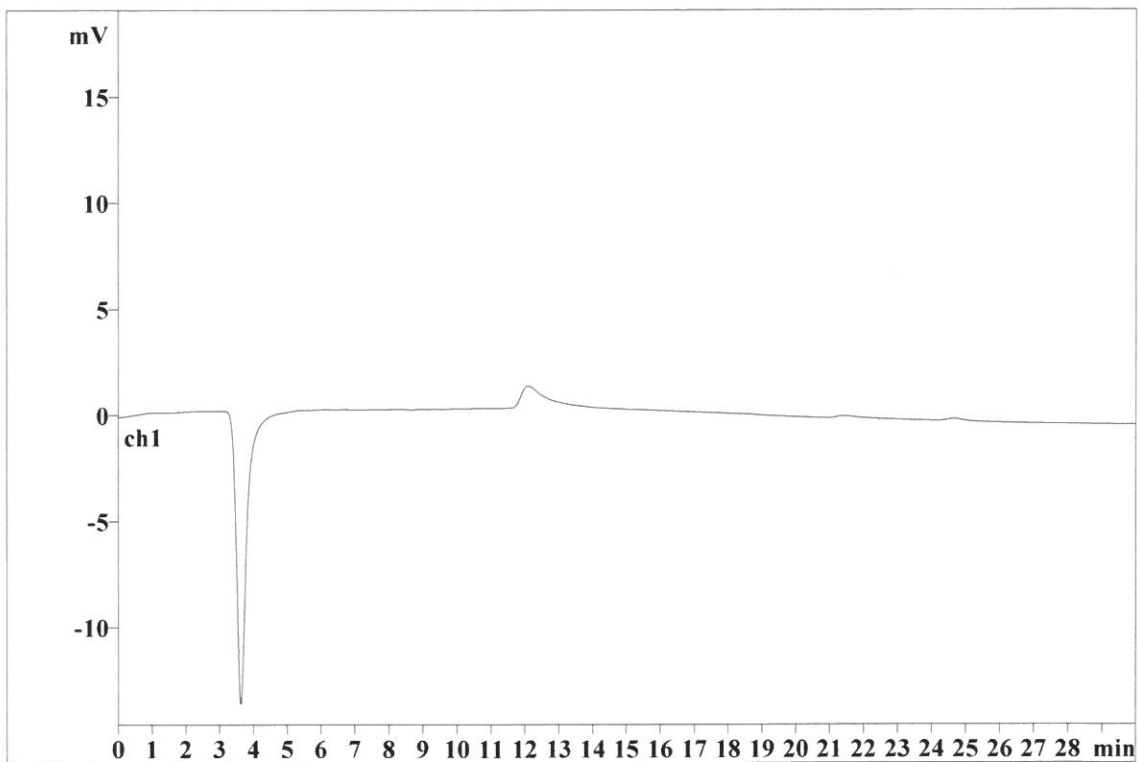

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/10/2020 9:15:23 AM
Printed by: wet


Ident: CCV
Analysis from: 8/7/2020 9:24:10 AM
File: _2020-08-07_

Last save: 8/7/2020 9:52:11 AM

Method: AnionsIC2-071420.mtw
Run operator: wet
Analysis number: 26767

Last save: 8/6/2020 3:11:2

SAMPLE: .
: AM/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

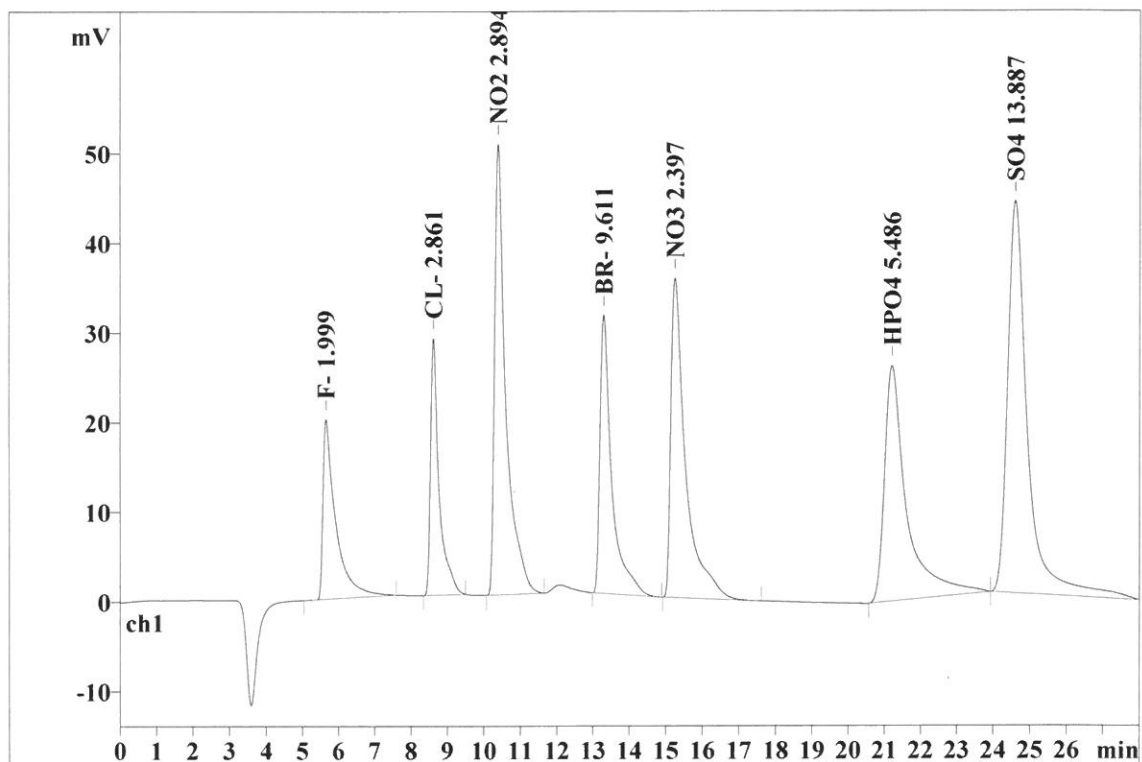

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.65	0.317	20.09	8.52	495.719	7.60
2	8.61	0.210	28.66	12.15	470.334	7.21
3	10.39	0.280	50.32	21.34	1087.292	16.67
4	13.30	0.289	31.07	13.17	698.352	10.70
5	15.26	0.357	35.68	15.13	989.433	15.17
6	21.22	0.530	26.28	11.14	1117.072	17.12
7	24.62	0.511	43.74	18.55	1665.965	25.54
7	28.00	0.356	235.83	100.00	6524.166	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/10/2020 9:15:35 AM
Printed by: wet


Ident: CCB
Analysis from: 8/7/2020 10:01:33 AM
File: _2020-08-07_

Last save: 8/7/2020 10:29:33 AM

Method: AnionsIC2-071420.mtw
Run operator: wet
Analysis number: 26768

Last save: 8/6/2020 3:11:2

SAMPLE:
: AM/AP
Vial number: 3
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

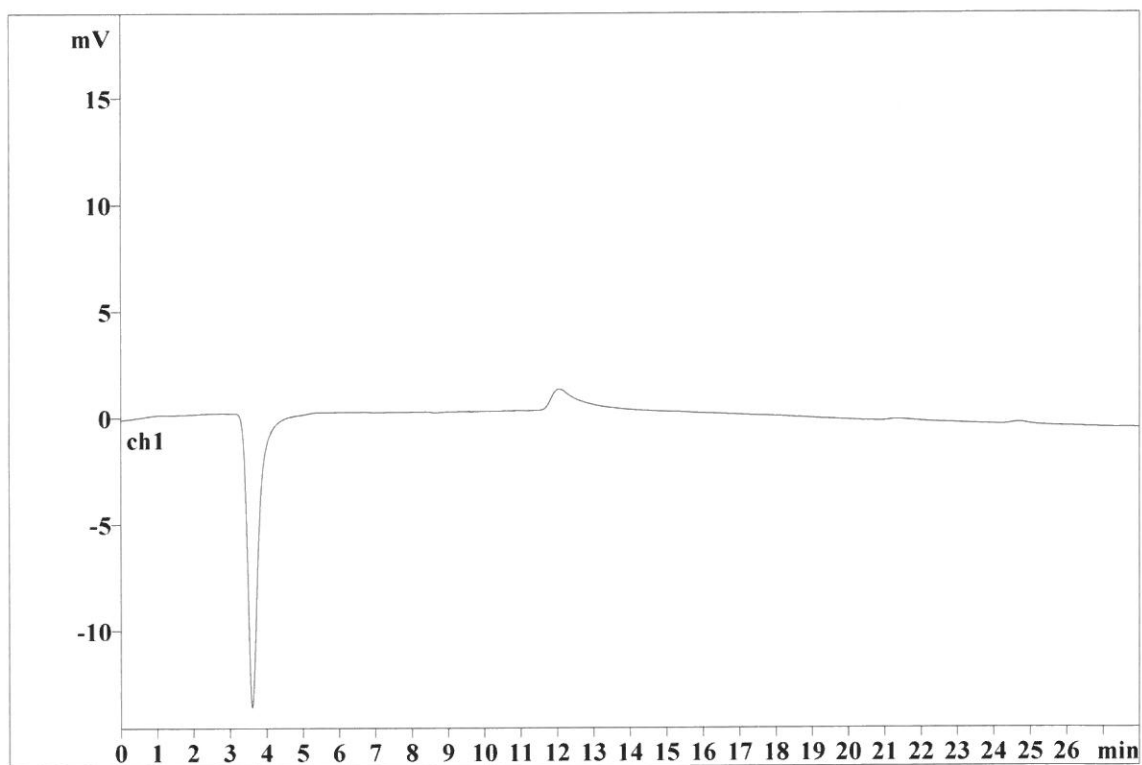

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/10/2020 9:15:42 AM
Printed by: wet


Ident: LB110423BLW
Analysis from: 8/7/2020 10:32:11 AM
File: _2020-08-07_

Last save: 8/7/2020 3:35:21 PM

Method: AnionsIC2-071420.mtw
Run operator: wet
Analysis number: 26769

Last save: 8/6/2020 3:11:2

SAMPLE:
: AM/AP
Vial number: 4
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

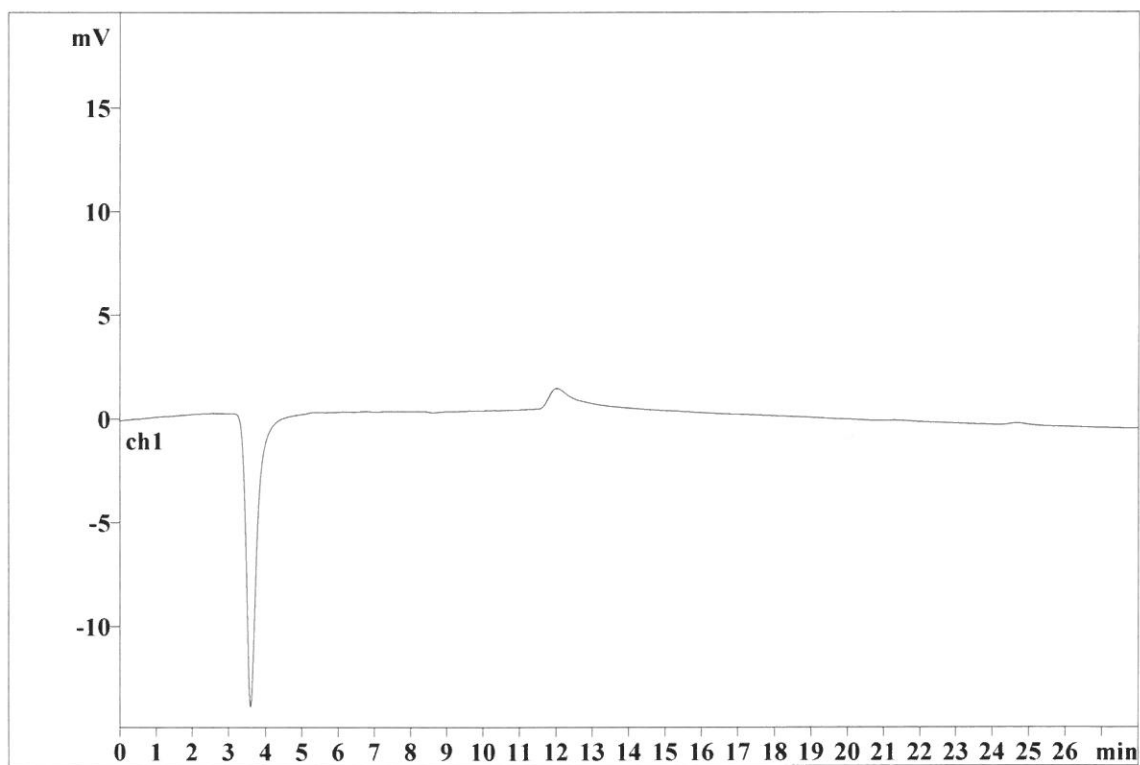

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/10/2020 9:15:50 AM
Printed by: wet


Ident: LB110423BSW
Analysis from: 8/7/2020 11:02:48 AM
File: _2020-08-07_

Last save: 8/7/2020 3:35:21 PM

Method: AnionsIC2-071420.mtw
Run operator: wet
Analysis number: 26770

Last save: 8/6/2020 3:11:2

SAMPLE:
: AM/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

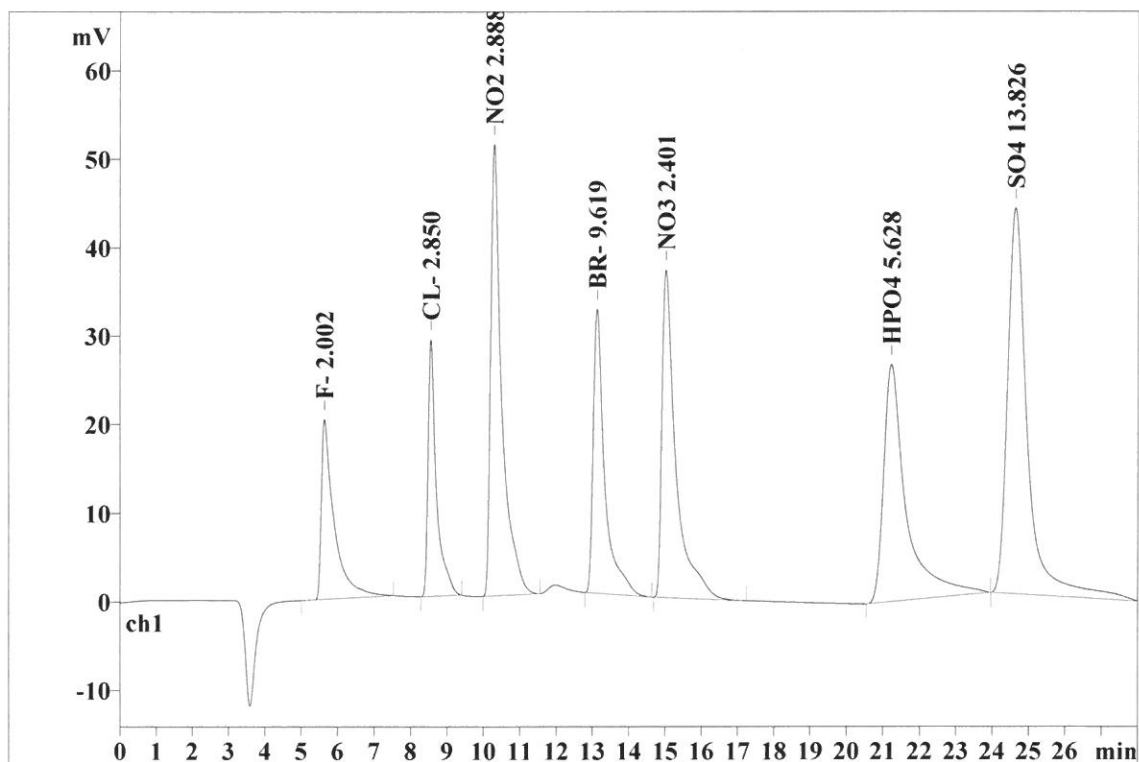

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.64	0.316	20.29	8.46	496.501	7.59
2	8.55	0.208	28.96	12.08	468.483	7.16
3	10.29	0.277	51.02	21.28	1084.829	16.58
4	13.12	0.280	32.09	13.39	698.901	10.68
5	15.02	0.345	37.01	15.44	991.273	15.15
6	21.23	0.531	26.75	11.16	1143.801	17.48
7	24.64	0.511	43.61	18.19	1658.481	25.35
7	28.00	0.353	239.74	99.99	6542.270	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/10/2020 9:16:07 AM
Printed by: wet


Ident: L3605-01
Analysis from: 8/7/2020 12:12:31 PM
File: _2020-08-07_

Last save: 8/7/2020 12:40:31 PM

Method: AnionsIC2-071420.mtw
Run operator: wet
Analysis number: 26772

Last save: 8/6/2020 3:11:2

SAMPLE:
: AM/AP
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

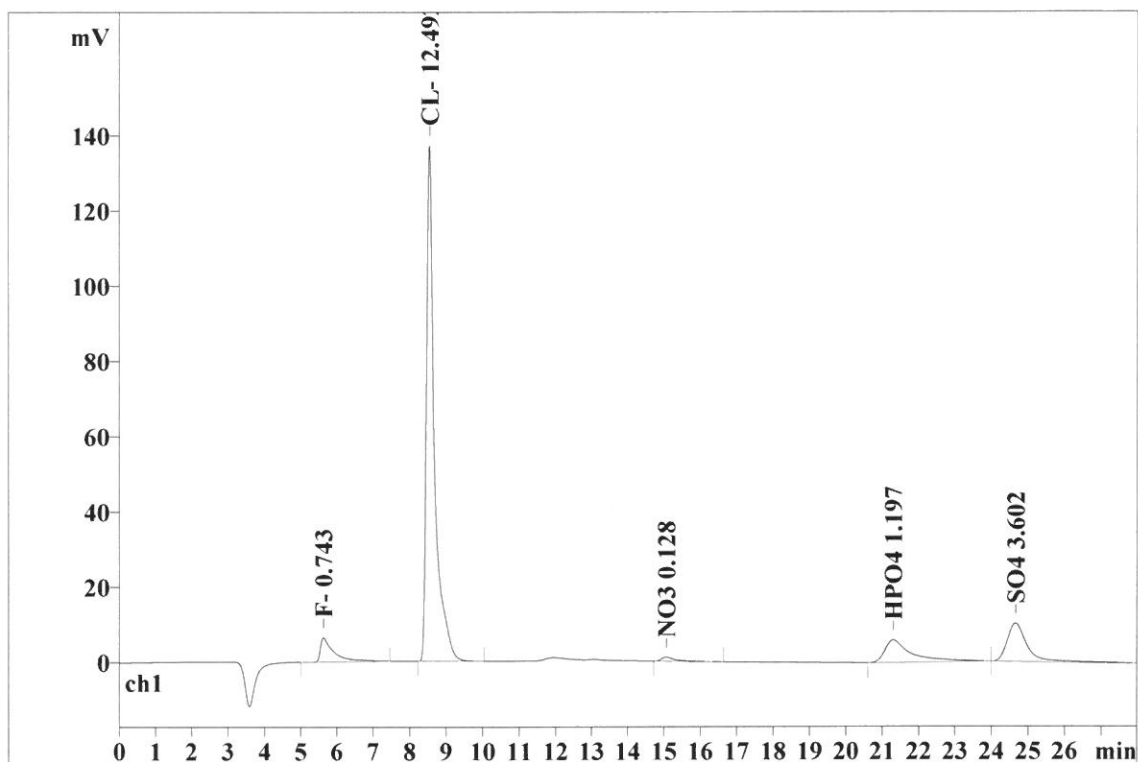

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.63	0.327	6.45	4.01	166.597	5.58
2	8.53	0.193	137.20	85.23	2086.741	69.93
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	15.07	0.349	1.09	0.68	29.261	0.98
6	21.30	0.626	6.00	3.72	308.428	10.34
7	24.66	0.521	10.22	6.35	392.831	13.17
7	28.00	0.288	160.96	99.99	2983.858	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/10/2020 9:16:15 AM
Printed by: wet


Ident: L3605-01DUP
Analysis from: 8/7/2020 12:43:09 PM
File: _2020-08-07_

Last save: 8/7/2020 1:11:10 PM

Method: AnionsIC2-071420.mtw
Run operator: wet
Analysis number: 26773

Last save: 8/6/2020 3:11:2

SAMPLE:
: AM/AP
Vial number: 10
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

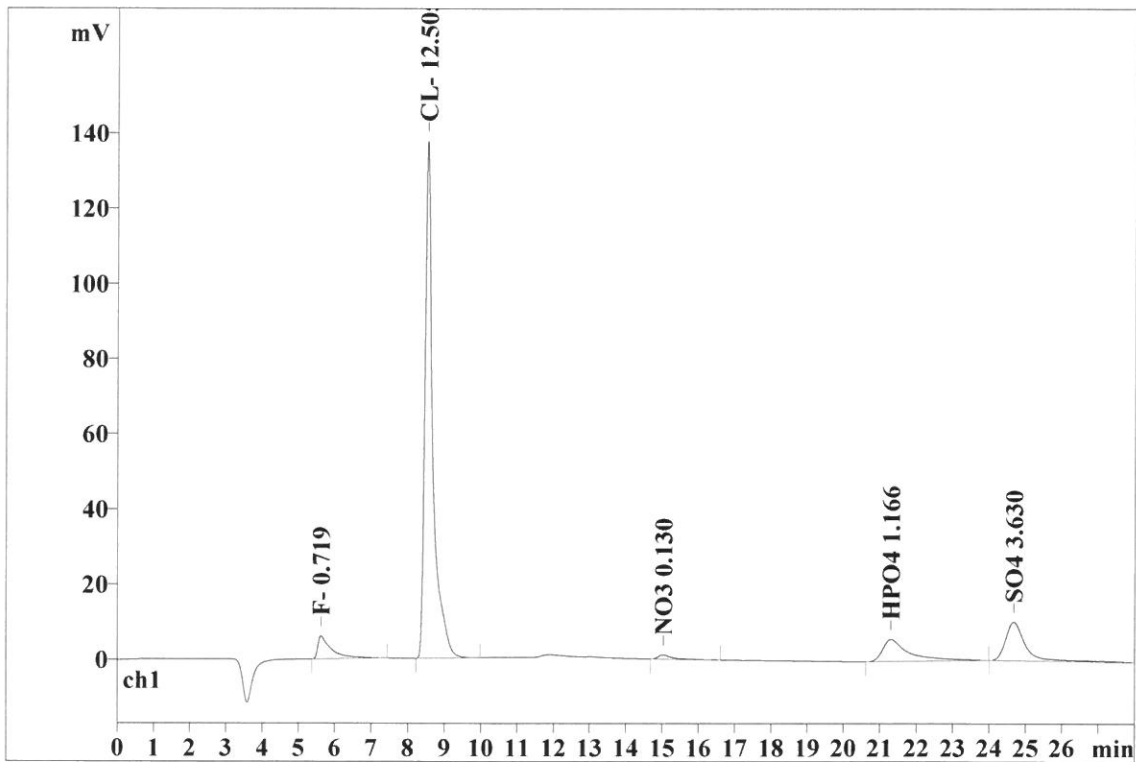

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.62	0.335	6.13	3.81	160.349	5.38
2	8.52	0.192	137.56	85.44	2088.928	70.14
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	15.03	0.350	1.12	0.70	29.888	1.00
6	21.31	0.624	5.91	3.67	302.642	10.16
7	24.68	0.521	10.27	6.38	396.372	13.31
7	28.00	0.289	160.99	100.00	2978.179	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/10/2020 9:16:22 AM
Printed by: wet


Ident: L3605-01MS
Analysis from: 8/7/2020 1:13:48 PM
File: _2020-08-07_

Last save: 8/7/2020 1:41:48 PM

Method: AnionsIC2-071420.mtw
Run operator: wet
Analysis number: 26774

Last save: 8/6/2020 3:11:2

SAMPLE:
: AM/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

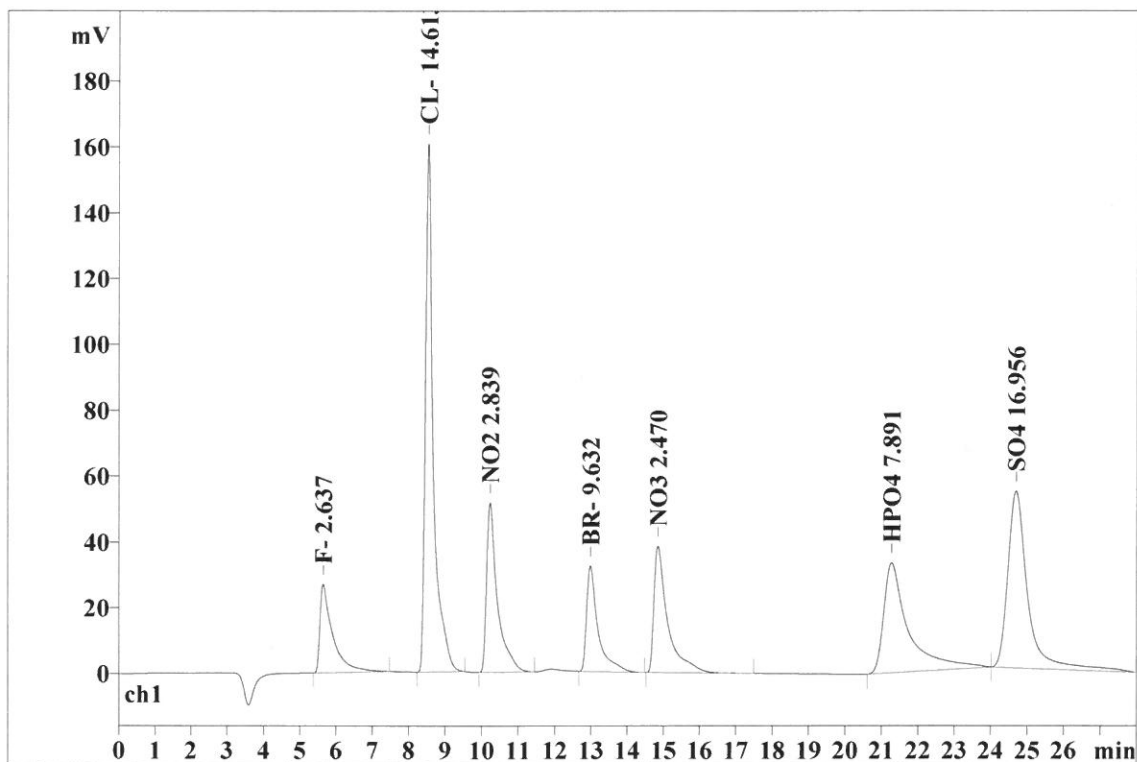

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.64	0.326	26.92	6.79	662.891	6.97
2	8.52	0.193	160.54	40.47	2442.702	25.69
3	10.22	0.269	51.47	12.97	1066.095	11.21
4	12.98	0.279	32.14	8.10	699.895	7.36
5	14.85	0.340	38.46	9.69	1020.535	10.73
6	21.27	0.569	33.44	8.43	1570.540	16.52
7	24.69	0.512	53.73	13.54	2045.900	21.52
7	28.00	0.355	396.70	100.00	9508.558	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/10/2020 9:16:28 AM
Printed by: wet


Ident: L3605-01MSD
Analysis from: 8/7/2020 1:44:26 PM
File: _2020-08-07_

Last save: 8/7/2020 2:12:26 PM

Method: AnionsIC2-071420.mtw
Run operator: wet
Analysis number: 26775

Last save: 8/6/2020 3:11:2

SAMPLE:
: AM/AP
Vial number: 12
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

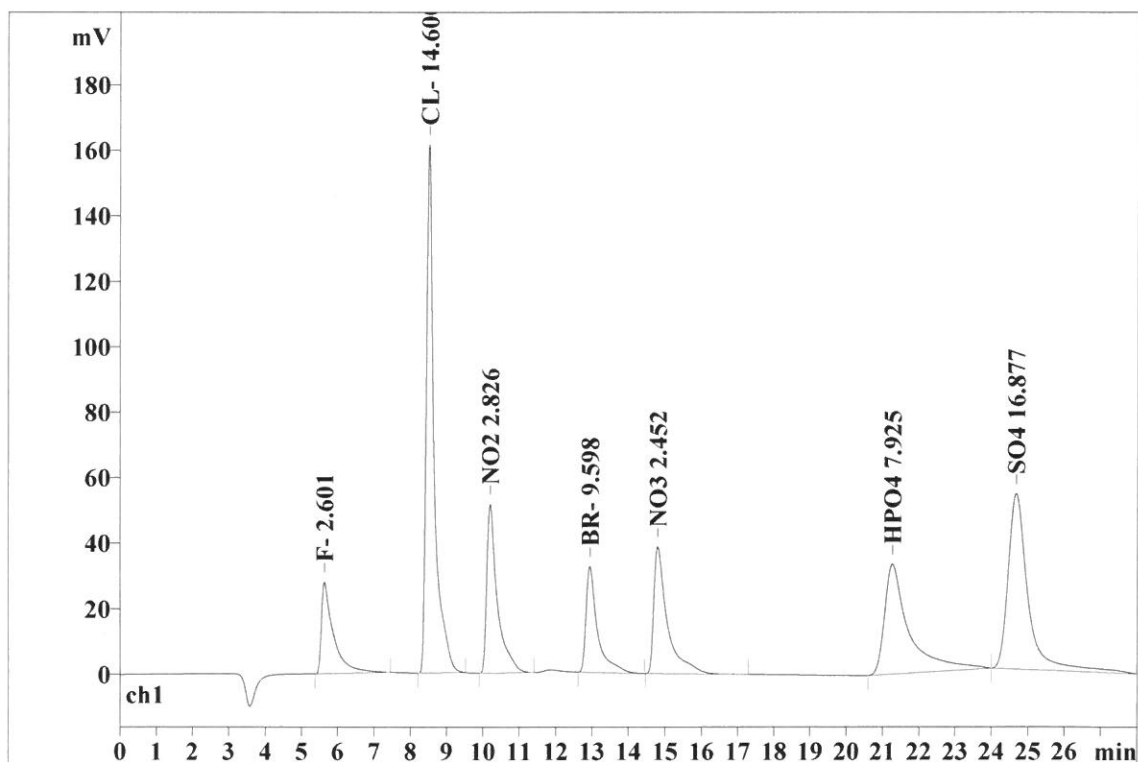

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.63	0.305	27.94	7.01	653.491	6.89
2	8.50	0.192	161.32	40.47	2440.455	25.75
3	10.20	0.269	51.45	12.91	1061.080	11.19
4	12.94	0.277	32.28	8.10	697.334	7.36
5	14.80	0.337	38.59	9.68	1012.870	10.69
6	21.26	0.569	33.50	8.41	1576.868	16.64
7	24.68	0.512	53.50	13.42	2036.125	21.48
7	28.00	0.352	398.59	100.00	9478.223	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/10/2020 9:17:39 AM
Printed by: wet


Ident: L3605-01DLX3
Analysis from: 8/7/2020 2:15:08 PM
File: _2020-08-07_

Last save: 8/7/2020 2:43:09 PM

Method: AnionsIC2-071420.mtw
Run operator: wet
Analysis number: 26776

Last save: 8/6/2020 3:11:2

SAMPLE:
: AM/AP
Vial number: 13
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

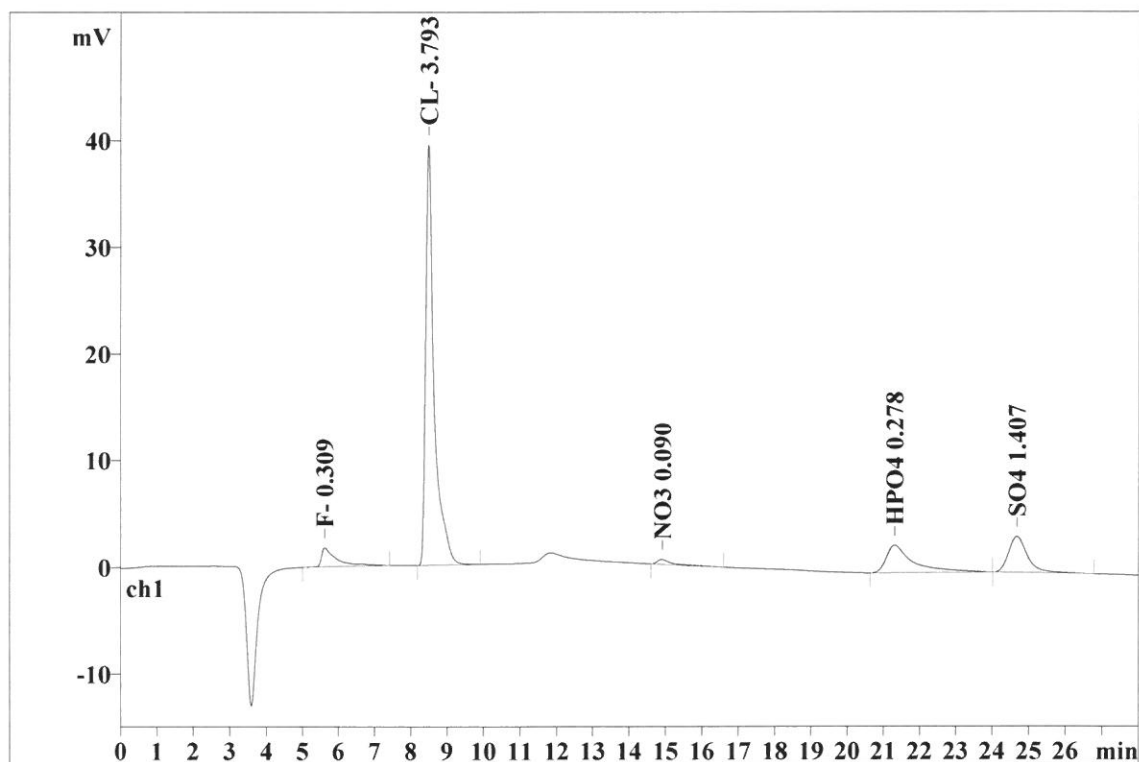

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.61	0.362	1.79	3.76	52.986	5.58
2	8.48	0.203	39.44	82.76	626.822	66.05
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	14.90	0.342	0.46	0.97	13.000	1.37
6	21.31	0.637	2.59	5.43	135.131	14.24
7	24.67	0.521	3.36	7.06	121.116	12.76
7	28.00	0.295	47.64	99.98	949.055	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/10/2020 9:17:46 AM
Printed by: wet


Ident: CCV
Analysis from: 8/7/2020 2:57:15 PM
File: _2020-08-07_

Last save: 8/7/2020 3:26:15 PM

Method: AnionsIC2-071420.mtw
Run operator: wet
Analysis number: 26777

Last save: 8/7/2020 3:24:3

SAMPLE:
: AM/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

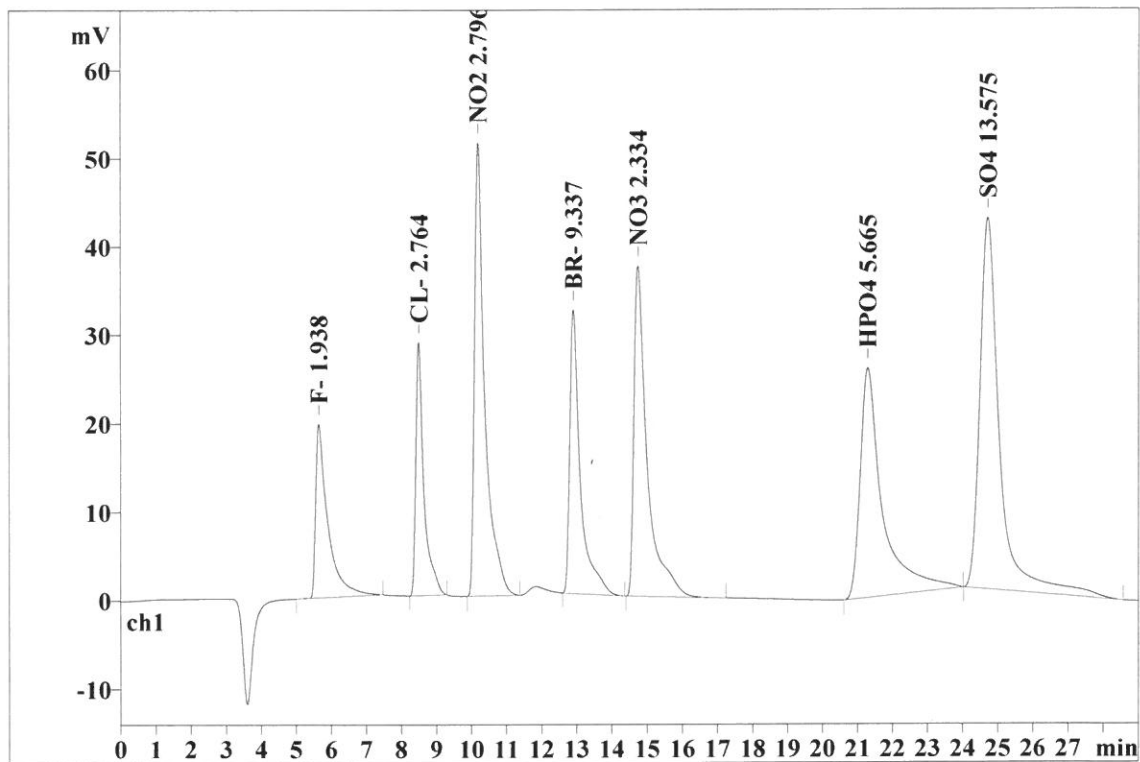

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.64	0.320	19.66	8.29	479.639	7.49
2	8.49	0.205	28.62	12.07	454.126	7.09
3	10.17	0.266	51.29	21.64	1049.329	16.39
4	12.90	0.271	32.08	13.54	677.842	10.59
5	14.74	0.330	37.39	15.78	962.753	15.04
6	21.29	0.544	25.96	10.95	1150.909	17.98
7	24.72	0.513	42.01	17.72	1627.398	25.42
7	29.00	0.350	237.00	100.00	6401.997	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/10/2020 9:17:54 AM
Printed by: wet


Ident: CCB
Analysis from: 8/7/2020 3:29:17 PM
File: _2020-08-07_

Last save: 8/7/2020 3:58:17 PM

Method: AnionsIC2-071420.mtw
Run operator: wet
Analysis number: 26778

Last save: 8/7/2020 3:24:3

SAMPLE:
: AM/AP
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

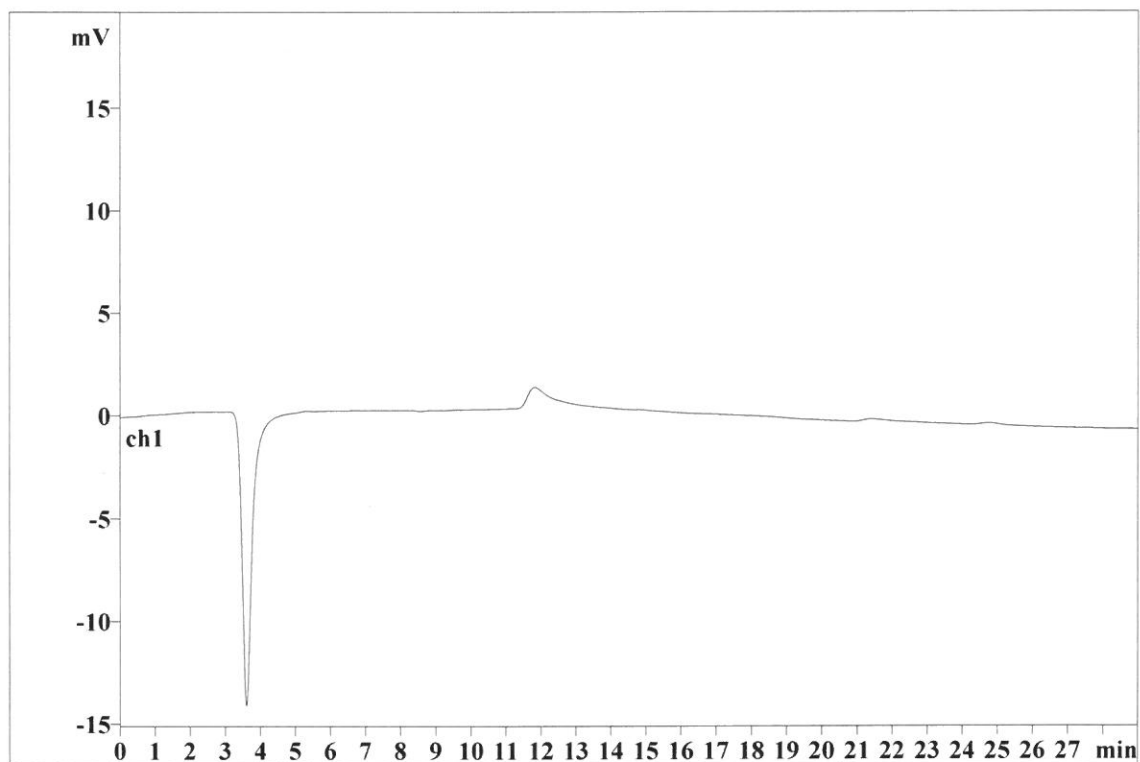

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/10/2020 9:18:01 AM
Printed by: wet


Ident: L3621-01
Analysis from: 8/7/2020 4:01:01 PM
File: _2020-08-07_

Last save: 8/7/2020 4:30:01 PM

Method: AnionsIC2-071420.mtw
Run operator: wet
Analysis number: 26779

Last save: 8/7/2020 3:24:3

SAMPLE:
: AM/AP
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

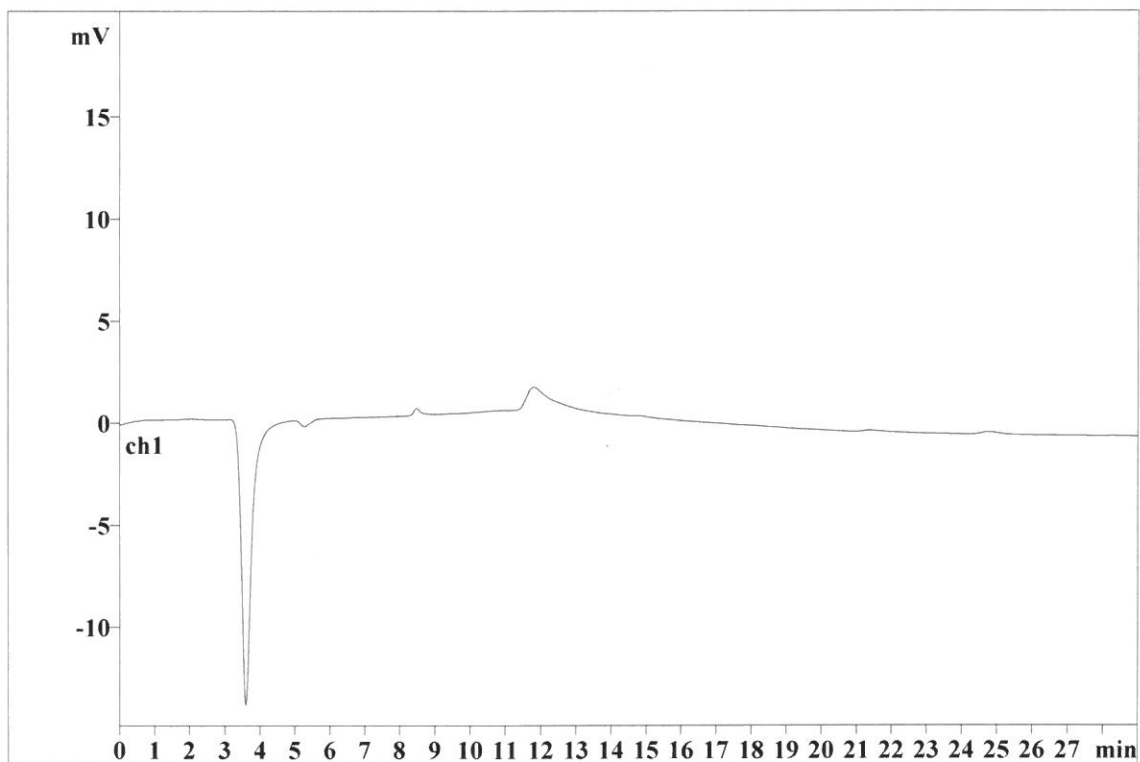

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 8/10/2020 9:18:10 AM
Printed by: wet


Ident: L3621-02
Analysis from: 8/7/2020 4:32:40 PM
File: _2020-08-07_

Last save: 8/7/2020 5:01:40 PM

Method: AnionsIC2-071420.mtw
Run operator: wet
Analysis number: 26780

Last save: 8/7/2020 3:24:3

SAMPLE:
: AM/AP
Vial number: 15
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

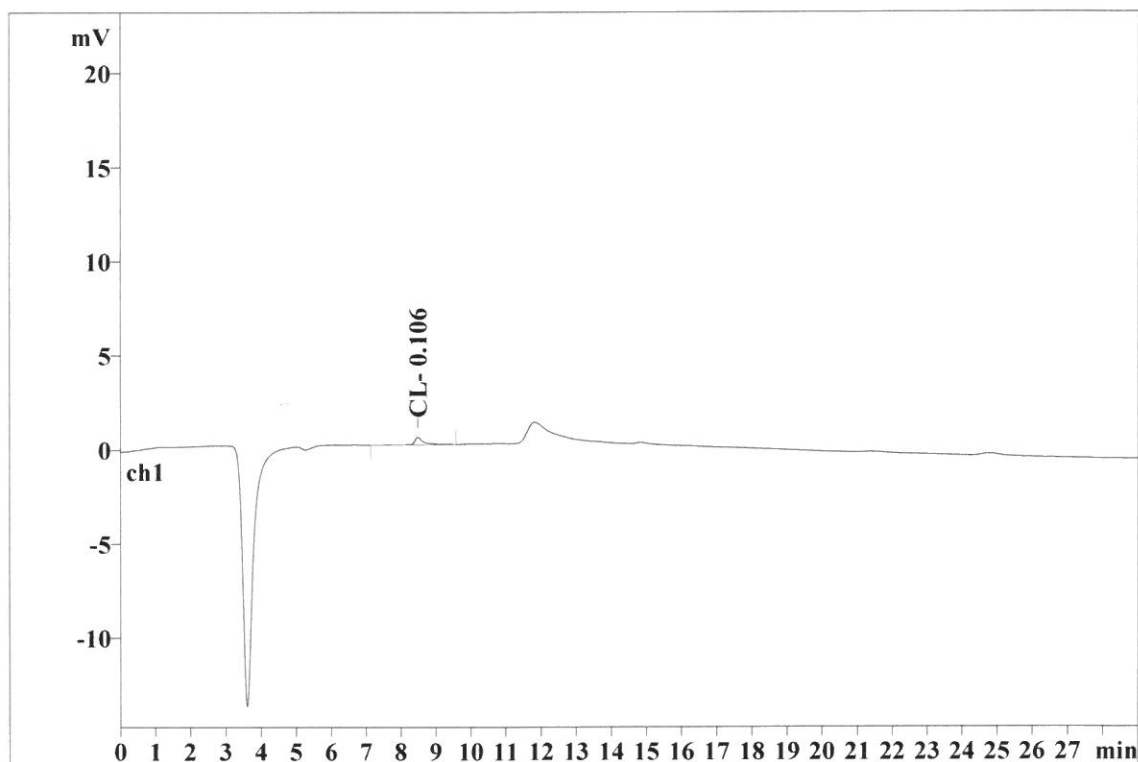

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.48	0.208	0.41	99.80	8.059	100.00
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	0.00	0.000	0.00	0.00	0.000	0.00
7	29.00	0.030	0.41	99.80	8.059	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/10/2020 9:18:41 AM
Printed by: wet


Ident: L3621-03
Analysis from: 8/7/2020 5:04:18 PM
File: _2020-08-07_

Last save: 8/10/2020 9:18:38 AM

Method: AnionsIC2-071420.mtw
Run operator: wet
Analysis number: 26781

Last save: 8/7/2020 3:24:3

SAMPLE:
: AM/AP
Vial number: 16
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

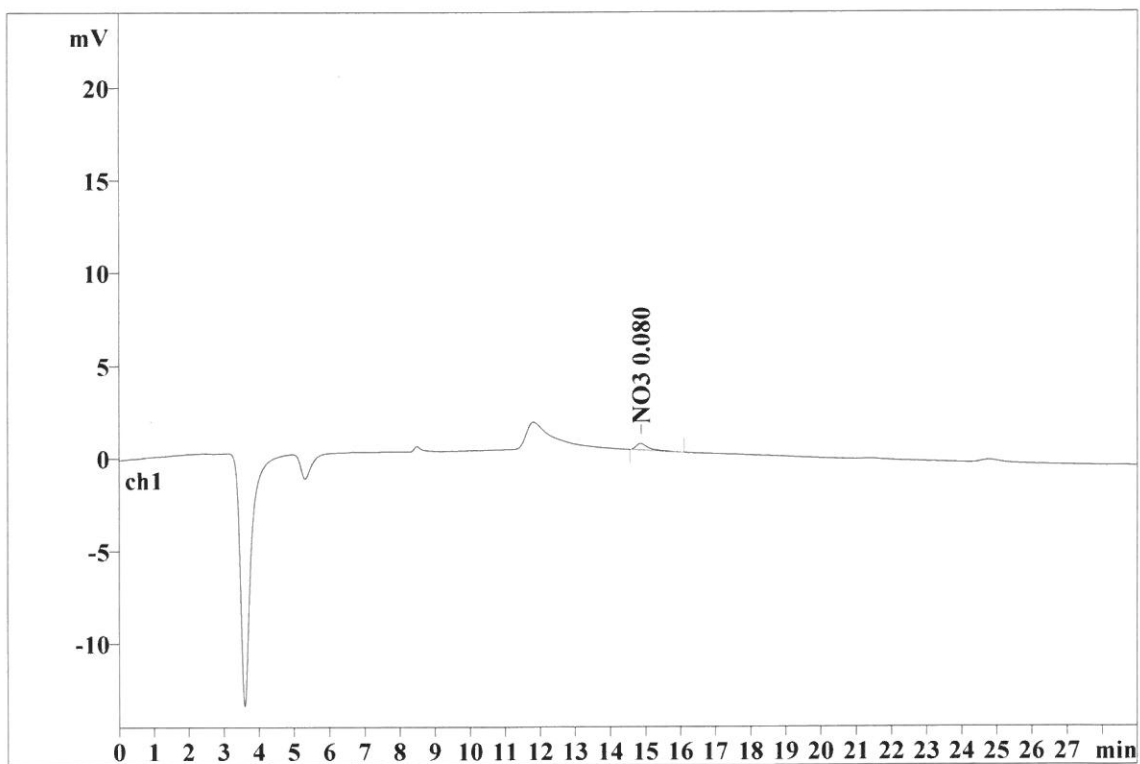

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	0.00	0.000	0.00	0.00	0.000	0.00
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	14.86	0.331	0.36	99.60	8.938	100.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	0.00	0.000	0.00	0.00	0.000	0.00
7	29.00	0.047	0.36	99.60	8.938	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/10/2020 9:18:48 AM
Printed by: wet


Ident: CCV
Analysis from: 8/7/2020 5:36:02 PM
File: _2020-08-07_

Last save: 8/7/2020 6:05:02 PM

Method: AnionsIC2-071420.mtw
Run operator: wet
Analysis number: 26782

Last save: 8/7/2020 3:24:3

SAMPLE:
: AM/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

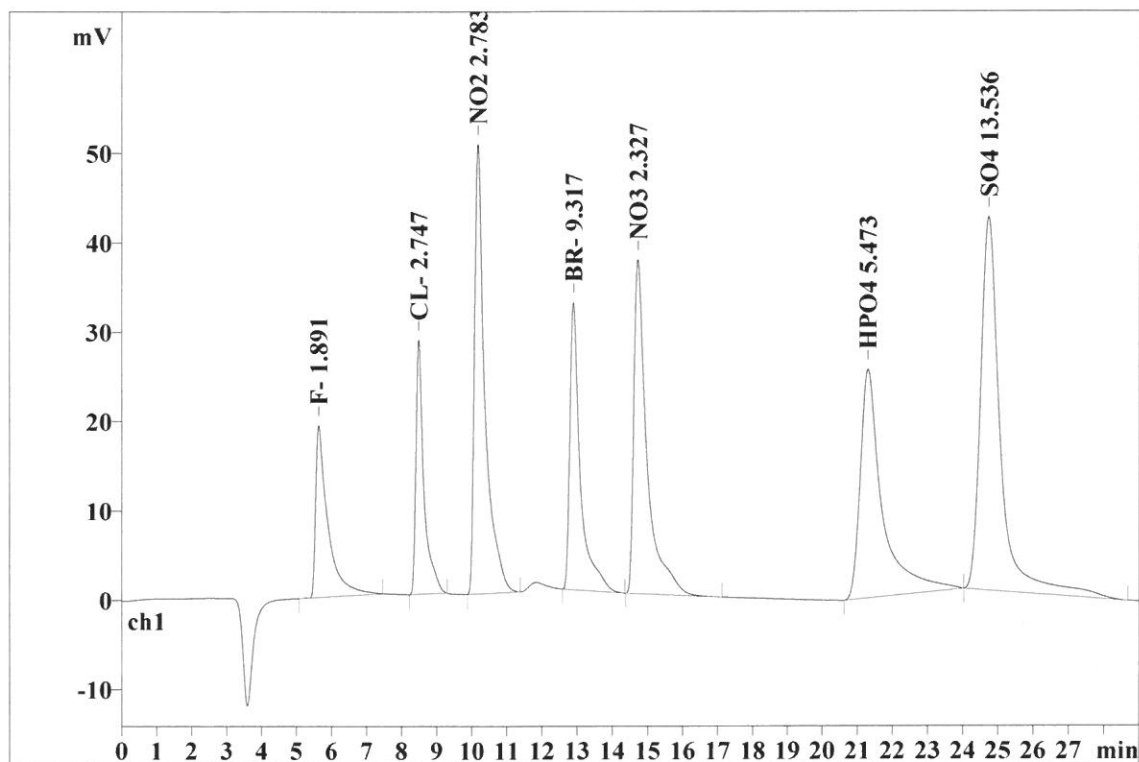

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.63	0.314	19.27	8.20	467.280	7.37
2	8.48	0.204	28.46	12.11	451.171	7.12
3	10.16	0.269	50.33	21.41	1044.320	16.48
4	12.89	0.269	32.18	13.69	676.363	10.67
5	14.72	0.328	37.38	15.90	959.821	15.15
6	21.29	0.538	25.61	10.90	1114.666	17.59
7	24.73	0.515	41.80	17.78	1622.564	25.61
7	29.00	0.348	235.03	100.00	6336.184	100.00

This report has been created by IC Net
METROHM LTD

Report date: 8/10/2020 9:18:55 AM
Printed by: wet


Ident: CCB
Analysis from: 8/7/2020 6:07:40 PM
File: _2020-08-07_

Last save: 8/7/2020 6:36:40 PM

Method: AnionsIC2-071420.mtw
Run operator: wet
Analysis number: 26783

Last save: 8/7/2020 3:24:3

SAMPLE:
: AM/AP
Vial number: 3
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

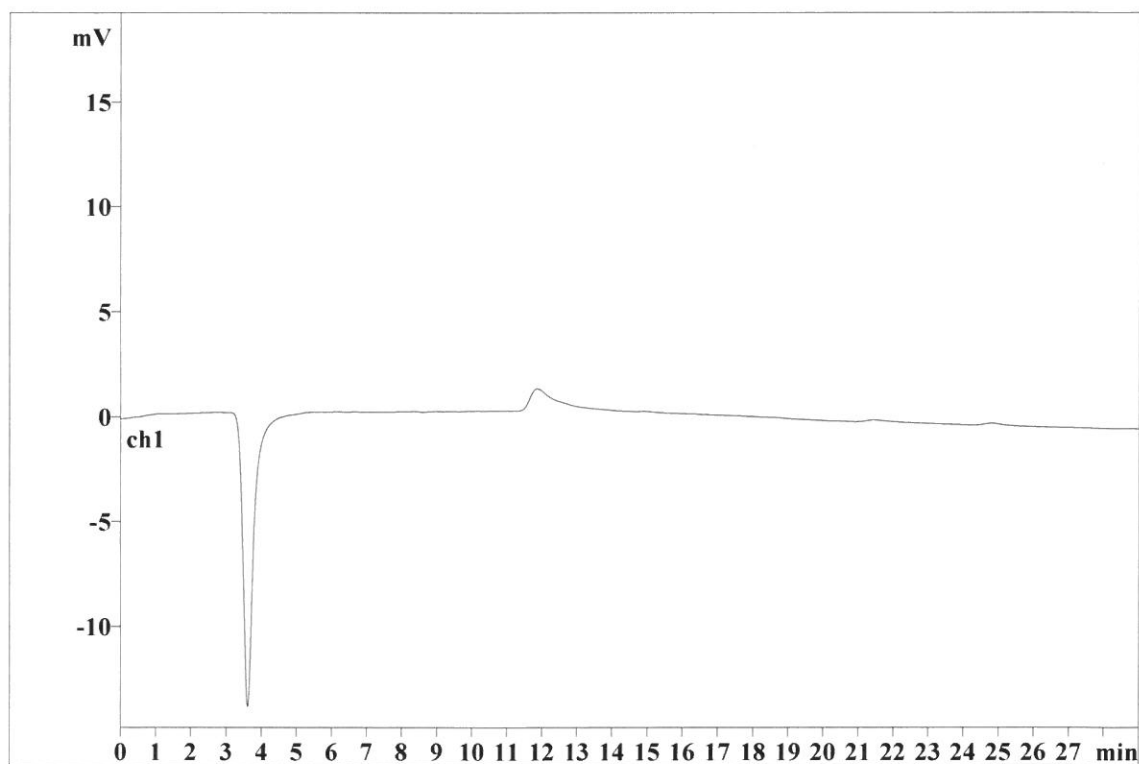

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD