

LB110460

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AM

Instrument ID : Konelab

8/10/2020 15:38

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.055	0.0	0.122	
ICB1	-0.333	0.0	0.002	
CCV1	238.542	0.0	0.302	
CCB1	-0.725	0.0	0.002	
PB130814BL	-0.378	0.0	0.002	
PB130814BS	95.650	0.0	0.123	
MIDPB130814	237.516	0.0	0.301	
L3589-01	-0.543	0.0	0.002	
L3589-01DUP	-0.699	0.0	0.002	
L3589-01MS	46.648	0.0	0.061	
L3589-01MSD	46.568	0.0	0.061	
CCV2	248.673	0.0	0.315	
CCB2	-0.615	0.0	0.002	

N	13
Mean	77.335
SD	99.9733
CV%	129.27

Aquakem v. 7.2AQ1

Results from time period:

Mon Aug 10 15:30:16 2020

Mon Aug 10 15:34:38 2020

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	-0.0205	µg/l	8/10/2020 12:35:08	
5.OPPBCN	A	Total CN	P	4.0052	µg/l	8/10/2020 12:35:09	
10PPBCN	A	Total CN	P	8.1516	µg/l	8/10/2020 12:35:10	
50PPBCN	A	Total CN	P	50.826	µg/l	8/10/2020 12:35:11	
100PPBCN	A	Total CN	P	101.0951	µg/l	8/10/2020 12:35:12	
250PPBCN	A	Total CN	P	252.3947	µg/l	8/10/2020 12:35:13	
500PPBCN	A	Total CN	P	498.5479	µg/l	8/10/2020 12:35:14	
ICV1	S	Total CN	P	95.0553	µg/l	8/10/2020 15:30:16	
ICB1	S	Total CN	P	-0.3328	µg/l	8/10/2020 15:30:17	
CCV1	S	Total CN	P	238.5423	µg/l	8/10/2020 15:30:18	
CCB1	S	Total CN	P	-0.7245	µg/l	8/10/2020 15:30:19	
PB130814BL	S	Total CN	P	-0.3783	µg/l	8/10/2020 15:30:20	
PB130814BS	S	Total CN	P	95.6499	µg/l	8/10/2020 15:30:21	
MIDPB130814	S	Total CN	P	237.5163	µg/l	8/10/2020 15:30:22	
L3589-01	S	Total CN	P	-0.5428	µg/l	8/10/2020 15:30:23	
L3589-01DUP	S	Total CN	P	-0.6992	µg/l	8/10/2020 15:30:24	
L3589-01MS	S	Total CN	P	46.6483	µg/l	8/10/2020 15:30:25	
L3589-01MSD	S	Total CN	P	46.5683	µg/l	8/10/2020 15:30:26	
CCV2	S	Total CN	P	248.6734	µg/l	8/10/2020 15:34:37	
CCB2	S	Total CN	P	-0.6153	µg/l	8/10/2020 15:34:38	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AM

Instrument ID : Konelab

8/10/2020 12:35

Test Total CN


Accepted 8/10/2020 12:35

Factor 796.2

Bias 0.003

Coeff. of det. 0.999931

Errors

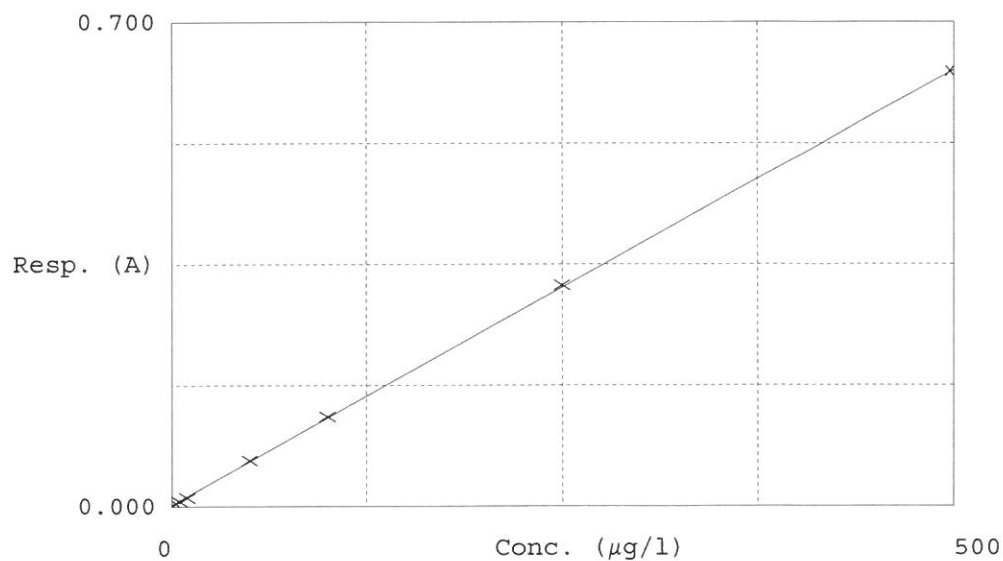

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-0.0205	0.0000	
2	5.0PPBCN	0.008	4.0052	5.0000	
3	10PPBCN	0.013	8.1516	10.0000	
4	50PPBCN	0.067	50.8260	50.0000	
5	100PPBCN	0.130	101.0951	100.0000	
6	250PPBCN	0.320	252.3947	250.0000	
7	500PPBCN	0.629	498.5479	500.0000	