

LB110484

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AM

Instrument ID : Konelab

8/11/2020 14:43

Test: Total CN

Sample Id	Result ^{ug/L}	Dil. 1 +	Response	Errors
ICV1	95.409	0.0	0.110	
ICB1	-0.554	0.0	0.002	
CCV1	243.580	0.0	0.278	
CCB1	-0.756	0.0	0.001	
PB130888BL	-0.923	0.0	0.001	
L3623-01	1.035	0.0	0.001	
L3623-01DUP	-0.627	0.0	0.001	
L3624-03	-1.289	0.0	0.001	
L3624-08	-0.892	0.0	0.001	
L3624-13	-0.942	0.0	0.001	
L3624-18	-1.124	0.0	0.001	
L3637-08	-0.784	0.0	0.001	
L3637-14	-0.935	0.0	0.001	
L3637-20	-0.567	0.0	0.001	
CCV2	251.865	0.0	0.287	
CCB2	-0.190	0.0	0.002	

N	16
Mean	36.265
SD	85.9604
CV%	237.04

LB110484

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AM

Instrument ID : Konelab

8/12/2020 9:01

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
CCV1	246.917	0.0	0.282	
CCB1	2.311	0.0	0.005	
L3624-07	-0.872	0.0	0.001	
L3624-12	-0.878	0.0	0.001	
L3624-17	-0.970	0.0	0.001	
L3625-01	-1.015	0.0	0.001	
L3623-03	-1.032	0.0	0.001	
L3624-02	-0.983	0.0	0.001	
CCV2	240.594	0.0	0.274	
CCB2	-1.007	0.0	0.001	
PB130887BL	-0.902	0.0	0.001	
PB130887BS	96.340	0.0	0.111	
LOWPB130887	9.563	0.0	0.013	
HIGHPB130887	487.175	0.0	0.553	
L3623-02	-0.390	0.0	0.002	
L3623-02DUP	-0.802	0.0	0.001	
L3623-02MS	35.290	0.0	0.042	
L3623-02MSD	35.557	0.0	0.042	
CCV3	249.772	0.0	0.285	
CCB3	-0.838	0.0	0.001	

N 20
Mean 69.692
SD 132.4541
CV% 190.06

L3623
AM
8/12/2020

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : AM

Instrument ID : Konelab

8/12/2020 17:05


Test Total CN

Accepted 8/11/2020 13:47

Factor 883.8
 Bias 0.002

Coeff. of det. 0.999985

Errors

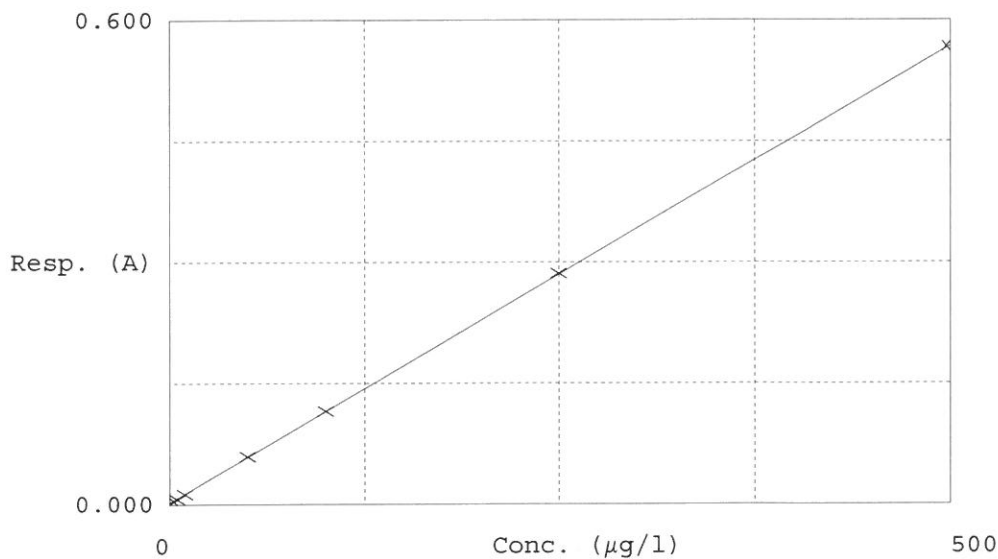

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	0.3809	0.0000	
2	5.0PPBCN	0.007	3.9717	5.0000	
3	10PPBCN	0.013	9.4695	10.0000	
4	50PPBCN	0.059	50.4515	50.0000	
5	100PPBCN	0.116	100.3121	100.0000	
6	250PPBCN	0.286	251.0018	250.0000	
7	500PPBCN	0.567	499.4124	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Tue Aug 11 15:35:46 2020

Tue Aug 11 17:43:18 2020

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	0.3809	µg/l	8/11/2020 13:30:34	
5.0PPBCN	A	Total CN	P	3.9717	µg/l	8/11/2020 13:30:35	
10PPBCN	A	Total CN	P	9.4695	µg/l	8/11/2020 13:30:36	
50PPBCN	A	Total CN	P	50.4515	µg/l	8/11/2020 13:30:37	
100PPBCN	A	Total CN	P	100.3121	µg/l	8/11/2020 13:30:38	
250PPBCN	A	Total CN	P	251.0018	µg/l	8/11/2020 13:30:39	
500PPBCN	A	Total CN	P	499.4124	µg/l	8/11/2020 13:30:40	
ICV1	S	Total CN	P	95.4092	µg/l	8/11/2020 14:17:30	
ICB1	S	Total CN	P	-0.5545	µg/l	8/11/2020 14:17:31	
CCV1	S	Total CN	P	246.9166	µg/l	8/11/2020 16:28:56	
CCB1	S	Total CN	P	2.3109	µg/l	8/11/2020 16:28:57	
L3624-07	S	Total CN	P	-0.872	µg/l	8/11/2020 16:28:58	
L3624-12	S	Total CN	P	-0.8784	µg/l	8/11/2020 16:28:59	
L3624-17	S	Total CN	P	-0.9698	µg/l	8/11/2020 16:29:00	
L3625-01	S	Total CN	P	-1.0151	µg/l	8/11/2020 16:29:01	
L3623-03	S	Total CN	P	-1.0317	µg/l	8/11/2020 17:10:31	
L3624-02	S	Total CN	P	-0.9834	µg/l	8/11/2020 17:10:32	
CCV2	S	Total CN	P	240.594	µg/l	8/11/2020 17:18:06	
CCB2	S	Total CN	P	-1.0069	µg/l	8/11/2020 17:18:07	
PB130887BL	S	Total CN	P	-0.9016	µg/l	8/11/2020 17:18:08	
PB130887BS	S	Total CN	P	96.3399	µg/l	8/11/2020 17:18:09	
LOWPB130887	S	Total CN	P	9.5633	µg/l	8/11/2020 17:18:10	
HIGHPB130887	S	Total CN	P	487.1753	µg/l	8/11/2020 17:18:11	
L3623-02	S	Total CN	P	-0.3902	µg/l	8/11/2020 17:18:12	
L3623-02DUP	S	Total CN	P	-0.8016	µg/l	8/11/2020 17:18:13	
L3623-02MS	S	Total CN	P	35.2895	µg/l	8/11/2020 17:18:14	
L3623-02MSD	S	Total CN	P	35.5566	µg/l	8/11/2020 17:18:15	
CCV3	S	Total CN	P	249.7724	µg/l	8/11/2020 17:43:17	
CCB3	S	Total CN	P	-0.8376	µg/l	8/11/2020 17:43:18	