

LB110590

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AM

Instrument ID : Konelab

8/18/2020 16:39

Test: Total CN

Sample Id	^{ug/L} Result	Dil. 1 +	Response	Errors
ICV1	98.948	0.0	0.107	
ICB1	0.112	0.0	0.001	
CCV1	245.462	0.0	0.264	
CCB1	0.148	0.0	0.001	
PB131051BL	0.169	0.0	0.001	
PB130051BS	98.804	0.0	0.107	
L3721-01	107.377	0.0	0.116	
L3721-01DUP	106.918	0.0	0.116	
L3721-01MS	133.081	0.0	0.144	
L3721-01MSD	133.046	0.0	0.144	
L3721-05	84.395	0.0	0.091	
L3721-06	3.118	0.0	0.004	
CCV2	258.235	0.0	0.278	
CCB2	0.309	0.0	0.001	

N	14
Mean	90.723
SD	86.2759
CV%	95.10

Aquakem v. 7.2AQ1

Results from time period:

Tue Aug 18 15:54:01 2020

Tue Aug 18 16:35:49 2020

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	-0.1761	µg/l	8/18/2020 12:09:11	
5.0PPBCN	A	Total CN	P	5.1482	µg/l	8/18/2020 12:09:12	
10PPBCN	A	Total CN	P	10.5303	µg/l	8/18/2020 12:09:13	
50PPBCN	A	Total CN	P	46.8547	µg/l	8/18/2020 12:09:14	
100PPBCN	A	Total CN	P	101.6781	µg/l	8/18/2020 12:09:15	
250PPBCN	A	Total CN	P	251.9959	µg/l	8/18/2020 12:09:16	
500PPBCN	A	Total CN	P	498.9688	µg/l	8/18/2020 12:09:17	
ICV1	S	Total CN	P	98.9484	µg/l	8/18/2020 15:54:01	
ICB1	S	Total CN	P	0.1117	µg/l	8/18/2020 15:54:02	
CCV1	S	Total CN	P	245.4615	µg/l	8/18/2020 16:31:56	
CCB1	S	Total CN	P	0.1481	µg/l	8/18/2020 16:31:57	
PB131051BL	S	Total CN	P	0.1687	µg/l	8/18/2020 16:31:58	
PB130051BS	S	Total CN	P	98.8044	µg/l	8/18/2020 16:31:59	
L3721-01	S	Total CN	P	107.3773	µg/l	8/18/2020 16:32:00	
L3721-01DUP	S	Total CN	P	106.9181	µg/l	8/18/2020 16:32:01	
L3721-01MS	S	Total CN	P	133.0806	µg/l	8/18/2020 16:32:04	
L3721-01MSD	S	Total CN	P	133.0459	µg/l	8/18/2020 16:32:05	
L3721-05	S	Total CN	P	84.395	µg/l	8/18/2020 16:32:06	
L3721-06	S	Total CN	P	3.1177	µg/l	8/18/2020 16:35:47	
CCV2	S	Total CN	P	258.2346	µg/l	8/18/2020 16:35:48	
CCB2	S	Total CN	P	0.3095	µg/l	8/18/2020 16:35:49	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AM

Instrument ID : Konelab

8/18/2020 12:29


Test Total CN

Accepted 8/18/2020 12:29

Factor 931.7
Bias 0.001

Coeff. of det. 0.999912

Errors

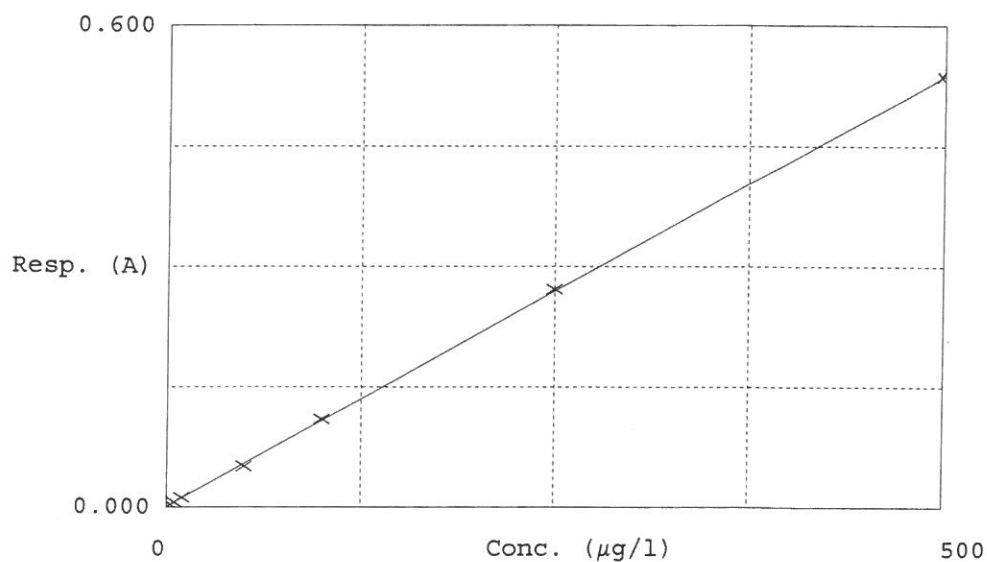

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	-0.1761	0.0000	
2	5.0PPBCN	0.006	5.1482	5.0000	
3	10PPBCN	0.012	10.5303	10.0000	
4	50PPBCN	0.051	46.8547	50.0000	
5	100PPBCN	0.110	101.6781	100.0000	
6	250PPBCN	0.271	251.9959	250.0000	
7	500PPBCN	0.536	498.9688	500.0000	