

LB110623

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AM

Instrument ID : Konelab

8/20/2020 12:16

Test: Total CN

Sample Id	Result ^{ug/L}	Dil. 1 +	Response	Errors
ICV1	99.106	0.0	0.074	
ICB1	-0.496	0.0	0.001	
CCV1	244.887	0.0	0.183	
CCB1	0.040	0.0	0.001	
PB131115BL	-0.586	0.0	0.001	
L3499-04	-0.537	0.0	0.001	
L3499-04DUP	-0.555	0.0	0.001	
L3504-12	-0.590	0.0	0.001	
L3507-12	-0.320	0.0	0.001	
L3742-04	-0.683	0.0	0.000	
L3742-08	-0.601	0.0	0.001	
L3502-15	-0.413	0.0	0.001	
CCV2	255.843	0.0	0.191	
CCB2	-0.373	0.0	0.001	

N	14
Mean	42.480
SD	91.9810
CV%	216.53

Aquakem v. 7.2AQ1

Results from time period:

Thu Aug 20 11:16:35 2020

Thu Aug 20 12:15:18 2020

Sample Id	Sam/Ctr/c/	Test short nan	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive CN	P	-0.3547	µg/l	8/20/2020 11:16:35	
5.0PPBCN	A	Reactive CN	P	4.1512	µg/l	8/20/2020 11:16:36	
10PPBCN	A	Reactive CN	P	9.4719	µg/l	8/20/2020 11:16:37	
50PPBCN	A	Reactive CN	P	49.725	µg/l	8/20/2020 11:16:38	
100PPBCN	A	Reactive CN	P	100.6783	µg/l	8/20/2020 11:16:39	
250PPBCN	A	Reactive CN	P	252.8348	µg/l	8/20/2020 11:16:40	
500PPBCN	A	Reactive CN	P	498.4935	µg/l	8/20/2020 11:16:41	
ICV1	S	Reactive CN	P	99.1058	µg/l	8/20/2020 11:58:57	
ICB1	S	Reactive CN	P	-0.4964	µg/l	8/20/2020 11:58:58	
CCV1	S	Reactive CN	P	244.8871	µg/l	8/20/2020 11:58:59	
CCB1	S	Reactive CN	P	0.0399	µg/l	8/20/2020 11:59:00	
PB131115BL	S	Reactive CN	P	-0.5857	µg/l	8/20/2020 11:59:01	
L3499-04	S	Reactive CN	P	-0.537	µg/l	8/20/2020 11:59:02	
L3499-04DUP	S	Reactive CN	P	-0.5554	µg/l	8/20/2020 11:59:03	
L3504-12	S	Reactive CN	P	-0.5898	µg/l	8/20/2020 11:59:05	
L3507-12	S	Reactive CN	P	-0.3204	µg/l	8/20/2020 11:59:06	
L3742-04	S	Reactive CN	P	-0.6833	µg/l	8/20/2020 11:59:07	
L3742-08	S	Reactive CN	P	-0.6006	µg/l	8/20/2020 12:02:51	
L3502-15	S	Reactive CN	P	-0.4134	µg/l	8/20/2020 12:13:04	
CCV2	S	Reactive CN	P	255.8434	µg/l	8/20/2020 12:15:17	
CCB2	S	Reactive CN	P	-0.3735	µg/l	8/20/2020 12:15:18	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AM

Instrument ID : Konelab

8/20/2020 11:18


Test Total CN

Accepted 8/20/2020 11:18

Factor 1348
Bias 0.001

Coeff. of det. 0.999942

Errors

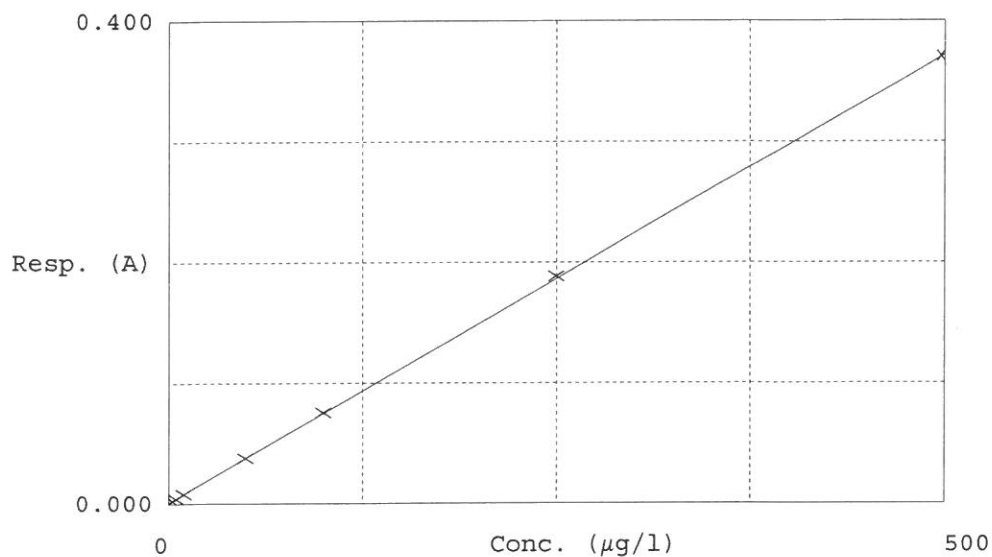

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	-0.3547	0.0000	
2	5.0PPBCN	0.004	4.1512	5.0000	
3	10PPBCN	0.008	9.4719	10.0000	
4	50PPBCN	0.038	49.7250	50.0000	
5	100PPBCN	0.076	100.6783	100.0000	
6	250PPBCN	0.188	252.8348	250.0000	
7	500PPBCN	0.371	498.4935	500.0000	