

LB110796

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AM

Instrument ID : Konelab

9/2/2020 14:18

Test: Total CN

Sample Id	Result ^{ug/L}	Dil. 1 +	Response	Errors
ICV1	97.680	0.0	0.085	
ICB1	0.747	0.0	0.001	
CCV1	242.597	0.0	0.210	
CCB1	0.665	0.0	0.001	
PB131382BL	0.363	0.0	0.001	
L3859-04	0.286	0.0	0.001	
L3859-04DUP	0.497	0.0	0.001	
L3866-05	0.536	0.0	0.001	
L3873-01	0.356	0.0	0.001	
PB131383BL	0.425	0.0	0.001	
L3858-02	0.407	0.0	0.001	
L3858-02DUP	0.623	0.0	0.001	
CCV2	254.957	0.0	0.221	
CCB2	0.699	0.0	0.001	

N	14
Mean	42.917
SD	90.9838
CV%	212.00

Aquakem v. 7.2AQ1

Results from time period:

Wed Sep 02 13:40:12 2020

Wed Sep 02 14:16:04 2020

Sample Id	Sam/Ctr/c	Test short name	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	0.3112	µg/l	9/2/2020 13:40:12	
5.OPPBCN	A	Reactive CN	P	4.9674	µg/l	9/2/2020 13:40:13	
10PPBCN	A	Reactive CN	P	9.9829	µg/l	9/2/2020 13:40:14	
50PPBCN	A	Reactive CN	P	50.9127	µg/l	9/2/2020 13:40:15	
100PPBCN	A	Reactive CN	P	99.3965	µg/l	9/2/2020 13:40:16	
250PPBCN	A	Reactive CN	P	248.7984	µg/l	9/2/2020 13:40:17	
500PPBCN	A	Reactive CN	P	500.6309	µg/l	9/2/2020 13:40:18	
ICV1	S	Reactive CN	P	97.6801	µg/l	9/2/2020 14:12:11	
ICB1	S	Reactive CN	P	0.7473	µg/l	9/2/2020 14:12:12	
CCV1	S	Reactive CN	P	242.5974	µg/l	9/2/2020 14:12:13	
CCB1	S	Reactive CN	P	0.6646	µg/l	9/2/2020 14:12:14	
PB131382BL	S	Reactive CN	P	0.3635	µg/l	9/2/2020 14:12:15	
L3859-04	S	Reactive CN	P	0.2858	µg/l	9/2/2020 14:12:16	
L3859-04DUP	S	Reactive CN	P	0.4966	µg/l	9/2/2020 14:12:17	
L3866-05	S	Reactive CN	P	0.5356	µg/l	9/2/2020 14:12:18	
L3873-01	S	Reactive CN	P	0.3556	µg/l	9/2/2020 14:12:19	
PB131383BL	S	Reactive CN	P	0.4251	µg/l	9/2/2020 14:12:20	
L3858-02	S	Reactive CN	P	0.4072	µg/l	9/2/2020 14:12:21	
L3858-02DUP	S	Reactive CN	P	0.6234	µg/l	9/2/2020 14:16:02	
CCV2	S	Reactive CN	P	254.9568	µg/l	9/2/2020 14:16:03	
CCB2	S	Reactive CN	P	0.699	µg/l	9/2/2020 14:16:04	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AM

Instrument ID : Konelab

9/2/2020 13:45


Test Total CN

Accepted 9/2/2020 13:45

Factor 1157
Bias 0

Coeff. of det. 0.999985

Errors

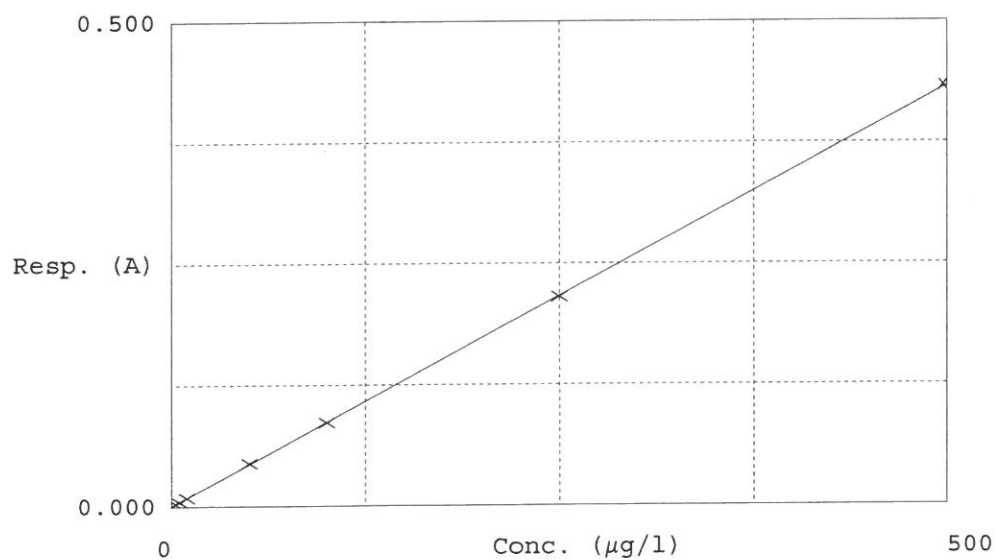

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	0.3112	0.0000	
2	5.0PPBCN	0.005	4.9674	5.0000	
3	10PPBCN	0.009	9.9829	10.0000	
4	50PPBCN	0.044	50.9127	50.0000	
5	100PPBCN	0.086	99.3965	100.0000	
6	250PPBCN	0.216	248.7984	250.0000	
7	500PPBCN	0.433	500.6309	500.0000	