

LB110945

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AM

Instrument ID : Konelab

9/14/2020 12:58

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.833	0.0	0.082	
ICB1	0.725	0.0	0.001	
CCV1	244.575	0.0	0.206	
CCB1	0.803	0.0	0.001	
PB131596BL	0.384	0.0	0.000	
L3941-04	0.447	0.0	0.000	
L3941-04DUP	0.314	0.0	0.000	
L3942-02	0.425	0.0	0.000	
L3953-02	0.479	0.0	0.000	
L3976-03	0.303	0.0	0.000	
L3863-04	0.531	0.0	0.000	
L3863-04DUP	0.086	0.0	0.000	
L3869-05	0.211	0.0	0.000	
L3941-01	0.484	0.0	0.000	
CCV2	244.427	0.0	0.206	
CCB2	0.821	0.0	0.001	
PB131597BL	0.163	0.0	0.000	
L3976-01	0.159	0.0	0.000	
L3976-02	0.307	0.0	0.000	
L3993-04	0.019	0.0	-0.000	
L3993-06	0.392	0.0	0.000	
L3993-10	0.108	0.0	0.000	
CCV3	254.327	0.0	0.214	
CCB3	0.082	0.0	0.000	

N	24
Mean	35.309
SD	84.3655
CV%	238.94

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AM

Instrument ID : Konelab

9/14/2020 11:46


Test Total CN

Accepted 9/14/2020 11:46

Factor 1186
Bias 0

Coeff. of det. 0.999994

Errors

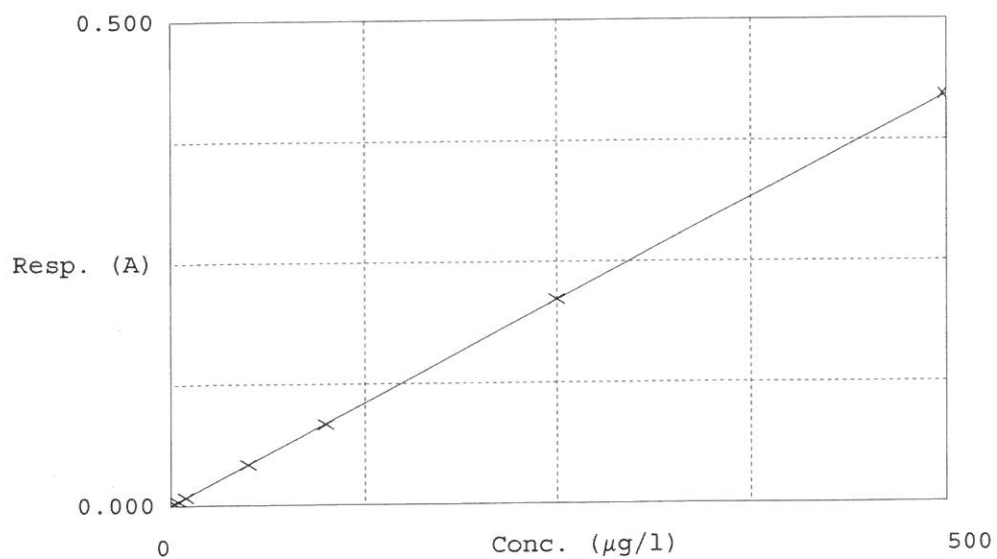

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.000	0.1524	0.0000	
2	5.0PPBCN	0.004	5.0797	5.0000	
3	10PPBCN	0.009	10.2324	10.0000	
4	50PPBCN	0.042	49.9519	50.0000	
5	100PPBCN	0.084	99.1222	100.0000	
6	250PPBCN	0.211	250.5731	250.0000	
7	500PPBCN	0.421	499.8884	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Mon Sep 14 11:41:55 2020

Mon Sep 14 12:50:54 2020

Sample Id	Sam/Ctr/c/	Test short nan	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	0.1524	µg/l	9/14/2020 11:41:55	
5.OPPBCN	A	Reactive CN	P	5.0797	µg/l	9/14/2020 11:41:56	
10PPBCN	A	Reactive CN	P	10.2324	µg/l	9/14/2020 11:41:57	
50PPBCN	A	Reactive CN	P	49.9519	µg/l	9/14/2020 11:41:58	
100PPBCN	A	Reactive CN	P	99.1222	µg/l	9/14/2020 11:41:59	
250PPBCN	A	Reactive CN	P	250.5731	µg/l	9/14/2020 11:42:00	
500PPBCN	A	Reactive CN	P	499.8884	µg/l	9/14/2020 11:42:01	
ICV1	S	Reactive CN	P	96.8326	µg/l	9/14/2020 12:39:55	
ICB1	S	Reactive CN	P	0.7255	µg/l	9/14/2020 12:39:56	
CCV1	S	Reactive CN	P	244.5748	µg/l	9/14/2020 12:39:57	
CCB1	S	Reactive CN	P	0.8027	µg/l	9/14/2020 12:39:58	
PB131596BL	S	Reactive CN	P	0.384	µg/l	9/14/2020 12:39:59	
L3941-04	S	Reactive CN	P	0.4466	µg/l	9/14/2020 12:40:00	
L3941-04DUP	S	Reactive CN	P	0.3139	µg/l	9/14/2020 12:40:01	
L3942-02	S	Reactive CN	P	0.4252	µg/l	9/14/2020 12:40:02	
L3953-02	S	Reactive CN	P	0.4787	µg/l	9/14/2020 12:40:03	
L3976-03	S	Reactive CN	P	0.3028	µg/l	9/14/2020 12:40:04	
L3863-04	S	Reactive CN	P	0.5309	µg/l	9/14/2020 12:40:05	
L3863-04DUP	S	Reactive CN	P	0.0856	µg/l	9/14/2020 12:47:30	
L3869-05	S	Reactive CN	P	0.2109	µg/l	9/14/2020 12:47:31	
L3941-01	S	Reactive CN	P	0.4842	µg/l	9/14/2020 12:47:32	
CCV2	S	Reactive CN	P	244.4274	µg/l	9/14/2020 12:47:33	
CCB2	S	Reactive CN	P	0.8213	µg/l	9/14/2020 12:47:34	
PB131597BL	S	Reactive CN	P	0.1632	µg/l	9/14/2020 12:47:35	
L3976-01	S	Reactive CN	P	0.1593	µg/l	9/14/2020 12:47:36	
L3976-02	S	Reactive CN	P	0.3072	µg/l	9/14/2020 12:47:37	
L3993-04	S	Reactive CN	P	0.0188	µg/l	9/14/2020 12:47:38	
L3993-06	S	Reactive CN	P	0.3917	µg/l	9/14/2020 12:47:39	
L3993-10	S	Reactive CN	P	0.1079	µg/l	9/14/2020 12:47:40	
CCV3	S	Reactive CN	P	254.3271	µg/l	9/14/2020 12:50:53	
CCB3	S	Reactive CN	P	0.082	µg/l	9/14/2020 12:50:54	