

LB111021

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092

Reviewed by : AM

Instrument ID : Konelab

9/17/2020 12:07

Test: Phenolics-

Sample Id	^{mg/L} Result	Dil. 1 +	Response	Errors
ICV1	0.979	0.0	0.106	
ICB1	-0.000	0.0	0.004	
CCV1	0.987	0.0	0.107	
CCB1	-0.007	0.0	0.003	
PB131564BL	0.001	0.0	0.004	
PB131564BS	0.985	0.0	0.106	
L3974-27	1.215	0.0	0.130	
CCV2	0.988	0.0	0.107	
CCB2	0.001	0.0	0.004	
N	9			
Mean	0.572			
SD	0.5487			
CV%	95.94			

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092

Reviewed by : AM

Instrument ID : Konelab

9/17/2020 11:20

Test Phenolics-


Accepted 9/17/2020 11:20

Factor 9.633

Bias 0.004

Coeff. of det. 0.999836

Errors

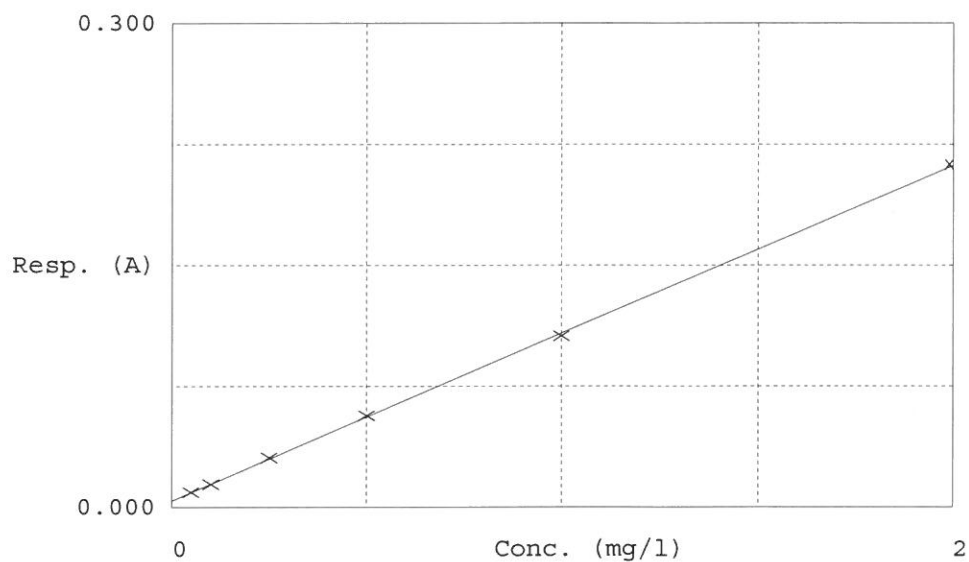

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.009	0.0502	0.0500	
2	Phenol-2	0.014	0.0972	0.1000	
3	Phenol-2	0.031	0.2561	0.2500	
4	Phenol-2	0.057	0.5079	0.5000	
5	Phenol-2	0.106	0.9823	1.0000	
6	Phenol-2	0.212	2.0062	2.0000	

Aquakem v. 7.2AQ1

Results from time period:

Thu Sep 17 11:19:24 2020

Thu Sep 17 11:59:06 2020

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0502	mg/l	9/17/2020 11:19:24	
0.1PPM	A	Phenolics-	P	0.0972	mg/l	9/17/2020 11:19:25	
0.25PPM	A	Phenolics-	P	0.2561	mg/l	9/17/2020 11:19:26	
0.5PPM	A	Phenolics-	P	0.5079	mg/l	9/17/2020 11:19:27	
1.0PPM	A	Phenolics-	P	0.9823	mg/l	9/17/2020 11:19:28	
2.0PPM	A	Phenolics-	P	2.0062	mg/l	9/17/2020 11:19:29	
ICV1	S	Phenolics-	P	0.9795	mg/l	9/17/2020 11:55:07	
ICB1	S	Phenolics-	P	0	mg/l	9/17/2020 11:55:08	
CCV1	S	Phenolics-	P	0.9867	mg/l	9/17/2020 11:55:09	
CCB1	S	Phenolics-	P	-0.0071	mg/l	9/17/2020 11:55:10	
PB131564BL	S	Phenolics-	P	0.0011	mg/l	9/17/2020 11:55:11	
PB131564BS	S	Phenolics-	P	0.9847	mg/l	9/17/2020 11:55:12	
L3974-27	S	Phenolics-	P	1.2145	mg/l	9/17/2020 11:55:15	
CCV2	S	Phenolics-	P	0.9876	mg/l	9/17/2020 11:55:17	
CCB2	S	Phenolics-	P	0.0007	mg/l	9/17/2020 11:55:18	