

LB111038

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AM

Instrument ID : Konelab

9/18/2020 11:46

Test: Total CN

Sample Id	Result ^{ug/L}	Dil. 1 +	Response	Errors
ICV1	96.622	0.0	0.080	
ICB1	2.291	0.0	0.002	
CCV1	241.659	0.0	0.200	
CCB1	-0.159	0.0	0.000	
PB131727BL	-0.406	0.0	-0.000	
L3870-10	-0.323	0.0	0.000	
L3870-10DUP	-0.204	0.0	0.000	
L3871-16	-0.195	0.0	0.000	
L3871-22	-0.300	0.0	0.000	
L4034-02	-0.255	0.0	0.000	
L4038-04	-0.332	0.0	0.000	
L4038-08	-0.566	0.0	-0.000	
L4038-10	-0.587	0.0	-0.000	
L4057-02	-0.104	0.0	0.000	
CCV2	243.661	0.0	0.201	
CCB2	-0.543	0.0	-0.000	
L4059-04	-0.327	0.0	0.000	
L4059-06	-0.289	0.0	0.000	
L4075-01	-0.255	0.0	0.000	
CCV3	253.928	0.0	0.210	
CCB3	-0.343	0.0	0.000	

N	21
Mean	39.665
SD	89.0370
CV%	224.47

Aquakem v. 7.2AQ1

Results from time period:

Fri Sep 18 11:19:12 2020

Fri Sep 18 11:45:25 2020

Sample Id	Sam/Ctr/c/	Test short nam	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-0.5892	µg/l	9/18/2020 9:41:39	
5.OPPBCN	A	Reactive CN	P	4.3432	µg/l	9/18/2020 9:41:40	
10PPBCN	A	Reactive CN	P	9.6015	µg/l	9/18/2020 9:41:41	
50PPBCN	A	Reactive CN	P	50.7002	µg/l	9/18/2020 9:41:42	
100PPBCN	A	Reactive CN	P	101.6237	µg/l	9/18/2020 9:41:43	
250PPBCN	A	Reactive CN	P	249.4017	µg/l	9/18/2020 9:41:44	
500PPBCN	A	Reactive CN	P	499.9189	µg/l	9/18/2020 9:41:45	
ICV1	S	Reactive CN	P	96.622	µg/l	9/18/2020 11:19:12	
ICB1	S	Reactive CN	P	2.2908	µg/l	9/18/2020 11:19:13	
CCV1	S	Reactive CN	P	241.6585	µg/l	9/18/2020 11:19:14	
CCB1	S	Reactive CN	P	-0.1588	µg/l	9/18/2020 11:19:15	
PB131727BL	S	Reactive CN	P	-0.4061	µg/l	9/18/2020 11:19:16	
L3870-10	S	Reactive CN	P	-0.3231	µg/l	9/18/2020 11:19:17	
L3870-10DUP	S	Reactive CN	P	-0.204	µg/l	9/18/2020 11:19:18	
L3871-16	S	Reactive CN	P	-0.1946	µg/l	9/18/2020 11:19:19	
L3871-22	S	Reactive CN	P	-0.3	µg/l	9/18/2020 11:19:20	
L4034-02	S	Reactive CN	P	-0.2546	µg/l	9/18/2020 11:19:21	
L4038-04	S	Reactive CN	P	-0.3322	µg/l	9/18/2020 11:19:22	
L4038-08	S	Reactive CN	P	-0.5665	µg/l	9/18/2020 11:26:19	
L4038-10	S	Reactive CN	P	-0.5875	µg/l	9/18/2020 11:26:20	
L4057-02	S	Reactive CN	P	-0.1037	µg/l	9/18/2020 11:26:21	
CCV2	S	Reactive CN	P	243.6611	µg/l	9/18/2020 11:26:22	
CCB2	S	Reactive CN	P	-0.5433	µg/l	9/18/2020 11:45:20	
L4059-04	S	Reactive CN	P	-0.3268	µg/l	9/18/2020 11:45:21	
L4059-06	S	Reactive CN	P	-0.2888	µg/l	9/18/2020 11:45:22	
L4075-01	S	Reactive CN	P	-0.2552	µg/l	9/18/2020 11:45:23	
CCV3	S	Reactive CN	P	253.9276	µg/l	9/18/2020 11:45:24	
CCB3	S	Reactive CN	P	-0.3427	µg/l	9/18/2020 11:45:25	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AM

Instrument ID : Konelab

9/18/2020 9:42

Test Total CN


Accepted 9/18/2020 9:42

Factor 1213

Bias 0

Coeff. of det. 0.999978

Errors

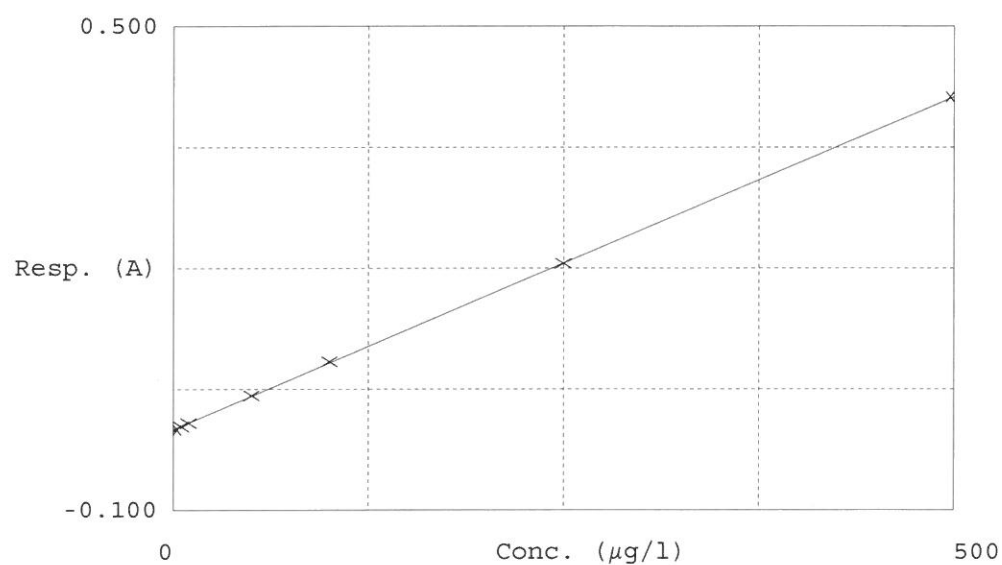

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	-0.000	-0.5892	0.0000	
2	5.0PPBCN	0.004	4.3432	5.0000	
3	10PPBCN	0.008	9.6015	10.0000	
4	50PPBCN	0.042	50.7002	50.0000	
5	100PPBCN	0.084	101.6237	100.0000	
6	250PPBCN	0.206	249.4017	250.0000	
7	500PPBCN	0.412	499.9189	500.0000	