

LB111045

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AM

Instrument ID : Konelab

9/18/2020 13:13

Test: Total CN

Sample Id	^{ug/L} Result	Dil. 1 +	Response	Errors
ICV1	97.077	0.0	0.080	
ICB1	-0.011	0.0	0.000	
CCV1	249.470	0.0	0.206	
CCB1	-0.067	0.0	0.000	
PB131705BL	-0.143	0.0	0.000	
PB131705BS	98.013	0.0	0.081	
MIDPB131705	240.751	0.0	0.199	
L4021-08	0.559	0.0	0.001	
L4025-01	0.711	0.0	0.001	
L4025-01DUP	0.776	0.0	0.001	
L4025-01MS	23.323	0.0	0.020	
L4025-01MSD	23.343	0.0	0.020	
CCV2	244.650	0.0	0.202	
CCB2	-0.048	0.0	0.000	

N	14
Mean	69.886
SD	100.6876
CV%	144.07

Aquakem v. 7.2AQ1

Results from time period:

Fri Sep 18 12:58:08 2020

Fri Sep 18 13:04:26 2020

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	-0.5892	µg/l	9/18/2020 9:41:39	
5.0PPBCN	A	Total CN	P	4.3432	µg/l	9/18/2020 9:41:40	
10PPBCN	A	Total CN	P	9.6015	µg/l	9/18/2020 9:41:41	
50PPBCN	A	Total CN	P	50.7002	µg/l	9/18/2020 9:41:42	
100PPBCN	A	Total CN	P	101.6237	µg/l	9/18/2020 9:41:43	
250PPBCN	A	Total CN	P	249.4017	µg/l	9/18/2020 9:41:44	
500PPBCN	A	Total CN	P	499.9189	µg/l	9/18/2020 9:41:45	
ICV1	S	Total CN	P	97.0766	µg/l	9/18/2020 12:58:08	
ICB1	S	Total CN	P	-0.0113	µg/l	9/18/2020 12:58:09	
CCV1	S	Total CN	P	249.4699	µg/l	9/18/2020 12:58:10	
CCB1	S	Total CN	P	-0.0665	µg/l	9/18/2020 12:58:11	
PB131705BL	S	Total CN	P	-0.1433	µg/l	9/18/2020 12:58:13	
PB131705BS	S	Total CN	P	98.0132	µg/l	9/18/2020 12:58:14	
MIDPB131705	S	Total CN	P	240.7508	µg/l	9/18/2020 12:58:15	
L4021-08	S	Total CN	P	0.5589	µg/l	9/18/2020 12:58:16	
L4025-01	S	Total CN	P	0.7106	µg/l	9/18/2020 12:58:17	
L4025-01DUP	S	Total CN	P	0.7757	µg/l	9/18/2020 12:58:18	
L4025-01MS	S	Total CN	P	23.3234	µg/l	9/18/2020 13:04:21	
L4025-01MSD	S	Total CN	P	23.3428	µg/l	9/18/2020 13:04:22	
CCV2	S	Total CN	P	244.6499	µg/l	9/18/2020 13:04:23	
CCB2	S	Total CN	P	-0.0481	µg/l	9/18/2020 13:04:24	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AM

Instrument ID : Konelab

9/18/2020 9:42


Test Total CN

Accepted 9/18/2020 9:42

Factor 1213
Bias 0

Coeff. of det. 0.999978

Errors

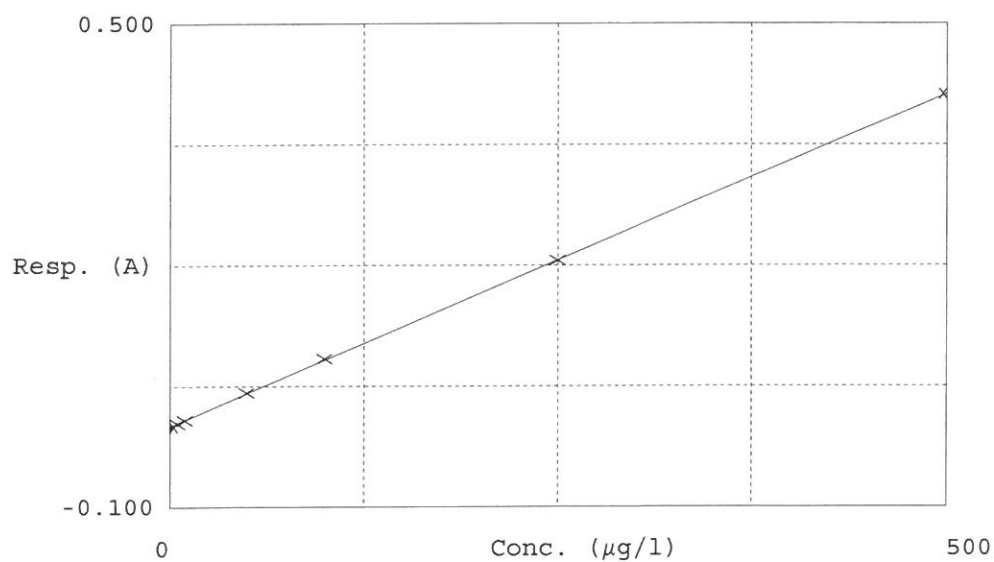

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	-0.000	-0.5892	0.0000	
2	5.0PPBCN	0.004	4.3432	5.0000	
3	10PPBCN	0.008	9.6015	10.0000	
4	50PPBCN	0.042	50.7002	50.0000	
5	100PPBCN	0.084	101.6237	100.0000	
6	250PPBCN	0.206	249.4017	250.0000	
7	500PPBCN	0.412	499.9189	500.0000	