

LB14087

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AM

Instrument ID : Konelab

9/22/2020 9:52

Test: Total CN

Sample Id	Result ^{ug/L}	Dil. 1 +	Response	Errors
ICV1	97.255	0.0	0.081	
ICB1	-0.719	0.0	0.000	
CCV1	244.351	0.0	0.201	
CCB1	-1.097	0.0	0.000	
PB131785BL	-1.329	0.0	-0.000	
L3864-15	-1.435	0.0	-0.000	
L3864-15DUP	-1.238	0.0	-0.000	
L3866-10	-1.222	0.0	0.000	
L3869-10	-1.484	0.0	-0.000	
L3872-10	-1.357	0.0	-0.000	
L4048-02	-1.206	0.0	0.000	
L4048-04	-1.200	0.0	0.000	
L4096-01	-0.995	0.0	0.000	
L4096-02	-0.686	0.0	0.000	
CCV2	247.652	0.0	0.203	
CCB2	-0.890	0.0	0.000	
L4101-02	-1.088	0.0	0.000	
L4104-04	-1.049	0.0	0.000	
L4104-08	-1.155	0.0	0.000	
L4104-10	-1.090	0.0	0.000	
PB131786BL	-1.196	0.0	0.000	
L4094-01	-1.055	0.0	0.000	
L4094-01DUP	-1.099	0.0	0.000	
CCV3	259.238	0.0	0.213	
CCB3	-1.022	0.0	0.000	

N	25
Mean	32.995
SD	84.2890
CV%	255.46

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : AM

Instrument ID : Konelab

9/22/2020 9:06


Test Total CN

Accepted 9/22/2020 9:06

Factor 1223
 Bias 0.001

Coeff. of det. 0.999766

Errors

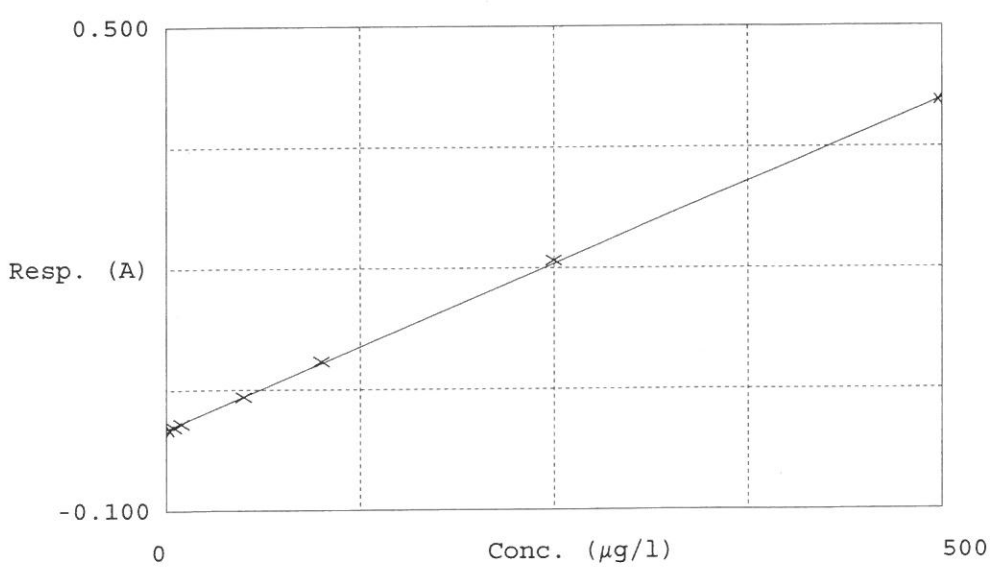

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	-0.000	-1.5123	0.0000	
2	5.0PPBCN	0.004	3.5660	5.0000	
3	10PPBCN	0.008	8.7052	10.0000	
4	50PPBCN	0.041	49.4881	50.0000	
5	100PPBCN	0.085	102.6467	100.0000	
6	250PPBCN	0.210	255.0884	250.0000	
7	500PPBCN	0.407	497.0179	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Tue Sep 22 09:04:48 2020

Tue Sep 22 09:50:28 2020

Sample Id	Sam/Ctr/c	Test short name	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive CN	P	-1.5123	µg/l	9/22/2020 9:04:48	
5.0PPBCN	A	Reactive CN	P	3.566	µg/l	9/22/2020 9:04:49	
10PPBCN	A	Reactive CN	P	8.7052	µg/l	9/22/2020 9:04:50	
50PPBCN	A	Reactive CN	P	49.4881	µg/l	9/22/2020 9:04:51	
100PPBCN	A	Reactive CN	P	102.6467	µg/l	9/22/2020 9:04:52	
250PPBCN	A	Reactive CN	P	255.0884	µg/l	9/22/2020 9:04:53	
500PPBCN	A	Reactive CN	P	497.0179	µg/l	9/22/2020 9:04:54	
ICV1	S	Reactive CN	P	97.2546	µg/l	9/22/2020 9:39:00	
ICB1	S	Reactive CN	P	-0.7187	µg/l	9/22/2020 9:39:01	
CCV1	S	Reactive CN	P	244.351	µg/l	9/22/2020 9:39:02	
CCB1	S	Reactive CN	P	-1.0965	µg/l	9/22/2020 9:39:03	
PB131785BL	S	Reactive CN	P	-1.3293	µg/l	9/22/2020 9:39:04	
L3864-15	S	Reactive CN	P	-1.4355	µg/l	9/22/2020 9:39:05	
L3864-15DUP	S	Reactive CN	P	-1.2383	µg/l	9/22/2020 9:39:06	
L3866-10	S	Reactive CN	P	-1.2217	µg/l	9/22/2020 9:39:07	
L3869-10	S	Reactive CN	P	-1.4844	µg/l	9/22/2020 9:39:08	
L3872-10	S	Reactive CN	P	-1.3572	µg/l	9/22/2020 9:39:09	
L4048-02	S	Reactive CN	P	-1.2056	µg/l	9/22/2020 9:39:10	
L4048-04	S	Reactive CN	P	-1.1998	µg/l	9/22/2020 9:46:35	
L4096-01	S	Reactive CN	P	-0.9945	µg/l	9/22/2020 9:46:36	
L4096-02	S	Reactive CN	P	-0.686	µg/l	9/22/2020 9:46:37	
CCV2	S	Reactive CN	P	247.6516	µg/l	9/22/2020 9:46:38	
CCB2	S	Reactive CN	P	-0.8901	µg/l	9/22/2020 9:46:39	
L4101-02	S	Reactive CN	P	-1.0884	µg/l	9/22/2020 9:46:40	
L4104-04	S	Reactive CN	P	-1.0494	µg/l	9/22/2020 9:46:41	
L4104-08	S	Reactive CN	P	-1.1546	µg/l	9/22/2020 9:46:42	
L4104-10	S	Reactive CN	P	-1.0899	µg/l	9/22/2020 9:46:43	
PB131786BL	S	Reactive CN	P	-1.1957	µg/l	9/22/2020 9:46:44	
L4094-01	S	Reactive CN	P	-1.0554	µg/l	9/22/2020 9:46:45	
L4094-01DUP	S	Reactive CN	P	-1.0985	µg/l	9/22/2020 9:50:26	
CCV3	S	Reactive CN	P	259.2379	µg/l	9/22/2020 9:50:27	
CCB3	S	Reactive CN	P	-1.0221	µg/l	9/22/2020 9:50:28	