

LB111386

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AM

Instrument ID : Konelab

10/8/2020 16:02

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.997	0.0	0.109	
ICB1	0.006	0.0	0.006	
CCV1	1.000	0.0	0.109	
CCB1	0.008	0.0	0.006	
PB132157BL	0.012	0.0	0.007	
PB132157BS	0.996	0.0	0.109	
L4214-10	0.031	0.0	0.009	
L4214-11	0.047	0.0	0.010	
L4233-01	0.006	0.0	0.006	
L4233-01DUP	0.009	0.0	0.006	
L4233-01MS	1.020	0.0	0.112	
L4233-01MSD	1.017	0.0	0.111	
CCV2	0.991	0.0	0.109	
CCB2	0.010	0.0	0.006	

N	14
Mean	0.439
SD	0.5073
CV%	115.47

Aquakem v. 7.2AQ1

Results from time period:

Thu Oct 08 15:17:40 2020

Thu Oct 08 15:57:59 2020

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0556	mg/l	10/8/2020 15:17:40	
0.1PPM	A	Phenolics-	P	0.1031	mg/l	10/8/2020 15:17:41	
0.25PPM	A	Phenolics-	P	0.2534	mg/l	10/8/2020 15:17:42	
0.50PPM	A	Phenolics-	P	0.5055	mg/l	10/8/2020 15:17:43	
1.0PPM	A	Phenolics-	P	0.9691	mg/l	10/8/2020 15:17:44	
2.0PPM	A	Phenolics-	P	2.0134	mg/l	10/8/2020 15:17:45	
ICV1	S	Phenolics-	P	0.9973	mg/l	10/8/2020 15:47:55	
ICB1	S	Phenolics-	P	0.0062	mg/l	10/8/2020 15:47:56	
CCV1	S	Phenolics-	P	0.9996	mg/l	10/8/2020 15:47:58	
CCB1	S	Phenolics-	P	0.0076	mg/l	10/8/2020 15:48:00	
PB132157BL	S	Phenolics-	P	0.0119	mg/l	10/8/2020 15:48:02	
PB132157BS	S	Phenolics-	P	0.9963	mg/l	10/8/2020 15:48:03	
L4214-10	S	Phenolics-	P	0.0309	mg/l	10/8/2020 15:48:05	
L4214-11	S	Phenolics-	P	0.0473	mg/l	10/8/2020 15:57:49	
L4233-01	S	Phenolics-	P	0.0063	mg/l	10/8/2020 15:57:51	
L4233-01DUP	S	Phenolics-	P	0.0088	mg/l	10/8/2020 15:57:52	
L4233-01MS	S	Phenolics-	P	1.0201	mg/l	10/8/2020 15:57:53	
L4233-01MSD	S	Phenolics-	P	1.0172	mg/l	10/8/2020 15:57:54	
CCV2	S	Phenolics-	P	0.9913	mg/l	10/8/2020 15:57:57	
CCB2	S	Phenolics-	P	0.0101	mg/l	10/8/2020 15:57:58	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AM

Instrument ID : Konelab

10/8/2020 15:20


Test Phenolics-

Accepted 10/8/2020 15:20

Factor 9.609
Bias 0.005

Coeff. of det. 0.999565

Errors

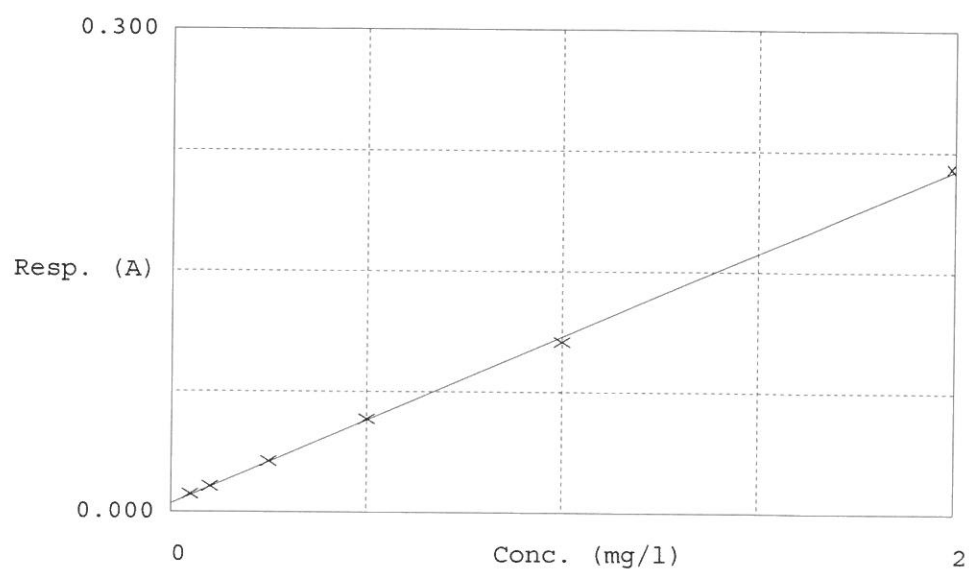

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.011	0.0556	0.0500	
2	Phenol-2	0.016	0.1031	0.1000	
3	Phenol-2	0.032	0.2534	0.2500	
4	Phenol-2	0.058	0.5055	0.5000	
5	Phenol-2	0.106	0.9691	1.0000	
6	Phenol-2	0.215	2.0134	2.0000	