

LB111389

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AM

Instrument ID : Konelab

10/8/2020 16:51

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.997	0.0	0.109	
ICB1	0.006	0.0	0.006	
CCV1	1.004	0.0	0.110	
CCB1	0.002	0.0	0.006	
PB132156BL	0.003	0.0	0.006	
PB132156BS	1.002	0.0	0.110	
L4214-01	0.026	0.0	0.008	
PB132158BL	0.006	0.0	0.006	
PB132158BS	1.004	0.0	0.110	
L4214-07	0.027	0.0	0.008	
L4214-08	0.047	0.0	0.010	
L4214-02	0.048	0.0	0.010	
CCV2	0.995	0.0	0.109	
CCB2	0.006	0.0	0.006	

N	14
Mean	0.369
SD	0.4882
CV%	132.18

Aquakem v. 7.2AQ1

Results from time period:

Thu Oct 08 16:36:01 2020

Thu Oct 08 16:48:48 2020

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0556	mg/l	10/8/2020 15:17:40	
0.1PPM	A	Phenolics-	P	0.1031	mg/l	10/8/2020 15:17:41	
0.25PPM	A	Phenolics-	P	0.2534	mg/l	10/8/2020 15:17:42	
0.50PPM	A	Phenolics-	P	0.5055	mg/l	10/8/2020 15:17:43	
1.0PPM	A	Phenolics-	P	0.9691	mg/l	10/8/2020 15:17:44	
2.0PPM	A	Phenolics-	P	2.0134	mg/l	10/8/2020 15:17:45	
ICV1	S	Phenolics-	P	0.9968	mg/l	10/8/2020 16:36:02	
ICB1	S	Phenolics-	P	0.0057	mg/l	10/8/2020 16:36:03	
CCV1	S	Phenolics-	P	1.0035	mg/l	10/8/2020 16:36:06	
CCB1	S	Phenolics-	P	0.0016	mg/l	10/8/2020 16:36:07	
PB132156BL	S	Phenolics-	P	0.0033	mg/l	10/8/2020 16:36:09	
PB132156BS	S	Phenolics-	P	1.0017	mg/l	10/8/2020 16:36:10	
L4214-01	S	Phenolics-	P	0.0258	mg/l	10/8/2020 16:36:11	
PB132158BL	S	Phenolics-	P	0.006	mg/l	10/8/2020 16:46:02	
PB132158BS	S	Phenolics-	P	1.0042	mg/l	10/8/2020 16:46:04	
L4214-07	S	Phenolics-	P	0.0268	mg/l	10/8/2020 16:46:06	
L4214-08	S	Phenolics-	P	0.0466	mg/l	10/8/2020 16:46:07	
L4214-02	S	Phenolics-	P	0.0479	mg/l	10/8/2020 16:46:08	
CCV2	S	Phenolics-	P	0.9949	mg/l	10/8/2020 16:46:10	
CCB2	S	Phenolics-	P	0.0061	mg/l	10/8/2020 16:46:11	

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : AM

Instrument ID : Konelab

10/8/2020 15:20


Test Phenolics-

Accepted 10/8/2020 15:20

Factor 9.609
 Bias 0.005

Coeff. of det. 0.999565

Errors

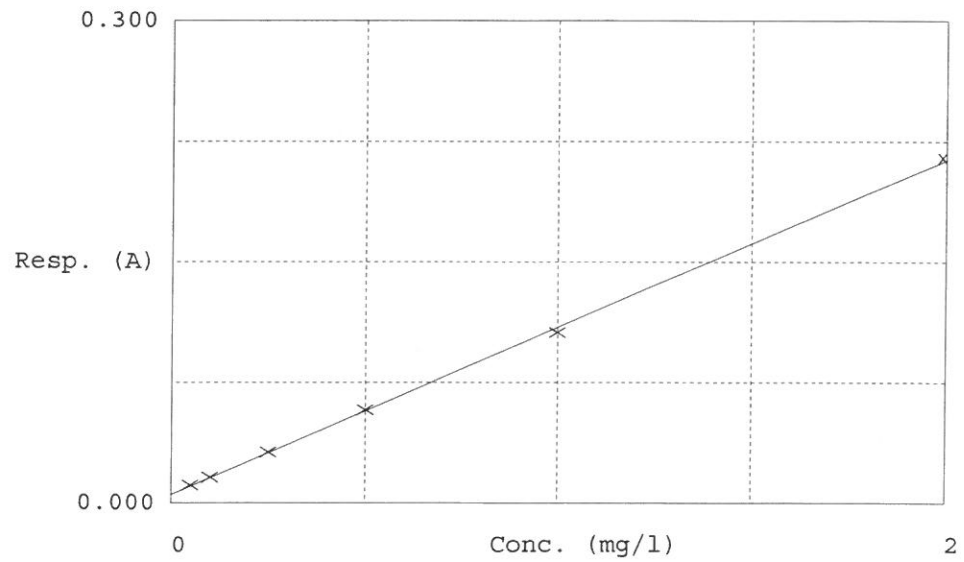

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.011	0.0556	0.0500	
2	Phenol-2	0.016	0.1031	0.1000	
3	Phenol-2	0.032	0.2534	0.2500	
4	Phenol-2	0.058	0.5055	0.5000	
5	Phenol-2	0.106	0.9691	1.0000	
6	Phenol-2	0.215	2.0134	2.0000	